

Effect of complex wavelet transform filter on thyroid tumor classification in three-dimensional ultrasound

*Original*

Effect of complex wavelet transform filter on thyroid tumor classification in three-dimensional ultrasound / U. R., Acharya; S. V., Sree; G., Swapna; S., Gupta; Molinari, Filippo; R., Garberoglio; A., Witkowska; J. S., Suri. - In: PROCEEDINGS OF THE INSTITUTION OF MECHANICAL ENGINEERS. PART H, JOURNAL OF ENGINEERING IN MEDICINE. - ISSN 0954-4119. - ELETTRONICO. - 227:H3(2013), pp. 284-292. [10.1177/0954411912472422]

*Availability:*

This version is available at: 11583/2512276 since:

*Publisher:*

SAGE

*Published*

DOI:10.1177/0954411912472422

*Terms of use:*

This article is made available under terms and conditions as specified in the corresponding bibliographic description in the repository

*Publisher copyright*

(Article begins on next page)

# Effect of Complex Wavelet Transform Filter on Thyroid Tumor Classification in 3D Ultrasound

U Rajendra Acharya<sup>1,2</sup>, G Swapna<sup>3</sup>, Savita Gupta<sup>4</sup>, S. Vinitha Sree<sup>5,\*</sup>, Filippo Molinari<sup>5</sup>, R. Garberoglio<sup>7</sup>,  
Agnieszka Witkowska<sup>8</sup>, Jasjit S. Suri<sup>9</sup>, *Sr. Member, IEEE, Fellow, AIMBE*

<sup>1</sup>Department of Electronics and Computer Engineering, Ngee Ann Polytechnic, Singapore

<sup>2</sup>Department of Biomedical Engineering, Faculty of Engineering, University of Malaya, 50603  
Kuala Lumpur, Malaysia

<sup>3</sup>Department of Applied Electronics and Instrumentation, Government Engineering College,  
Kozhikode, Kerala 673005, India

<sup>4</sup>Department of Computer Science and Engg., University Institute of Engineering and Technology  
(UIET), Panjab University, Chandigarh, India

<sup>5</sup>Global Biomedical Technologies Inc., CA, USA

<sup>6</sup>Biolab, Department of Electronics, Politecnico di Torino, Torino, Italy

<sup>7</sup>Scientific Foundation Mauriziana Onlus, Torino, Italy

<sup>8</sup>Department of Internal Medicine, Diabetology and Nephrology, Medical University of Silesia, Zabrze,  
Poland

<sup>9</sup>CTO, Global Biomedical Technologies, CA, USA and Biomedical Engineering Department,  
Idaho State University, (Affl.), ID, USA (email: [jsuri@comcast.net](mailto:jsuri@comcast.net))

\*Corresponding Author

Postal Address: U Rajendra Acharya; Email Address: [aru@np.edu.sg](mailto:aru@np.edu.sg)

## **Abstract**

Ultrasonography has great potential in differentiating malignant thyroid nodules from the benign ones. However, visual interpretation is limited by inter-observer variability, and further, the speckle distribution poses a challenge during the classification process. This paper thus presents an automated system for tumor classification in 3D Contrast-Enhanced Ultrasonography (CEUS) data sets. The system first processes the CEUS images using Complex Wavelet Transform (CWT) based filter to mitigate the effect of speckle noise. The Higher Order Spectra (HOS) features are then extracted and used as input for training and testing a Fuzzy classifier. In the off-line training system, HOS features are extracted from a set of images known as the training images. These HOS features along with the clinically assigned ground truth are used to train the classifier and obtain an estimate of the classifier or training parameters. The ground truth tells the class label of the image (i.e. whether the image belongs to a benign or malignant nodule). During the on-line testing phase, the estimated classifier parameters are applied on the HOS features which are extracted from the testing images, to predict their class labels. The predicted class labels are compared with their corresponding original ground truth to evaluate the performance of the classifier. Without utilizing the CWT filter, the Fuzzy classifier demonstrated an accuracy of 91.6%, while the accuracy significantly boosted to 99.1% by utilizing the CWT filter.

## **Keywords**

Thyroid nodule, Contrast Enhanced Ultrasound, Speckle, Complex Wavelet Transform, Benign, Malignant, Classification, Performance.

## Introduction

More than 50% of the adults have thyroid nodules, out of which 7% are likely to be malignant [1], and the malignancy incidence is increasing at the rate of 3% every year [2]. According to the National Cancer Institute, in the United States, in 2012, the estimated number of new thyroid cases is 56,460 and thyroid related cancer deaths is 1,780 [3]. Therefore, it is important to develop affordable and reliable diagnostic modalities or protocols for better thyroid malignancy management. Medical image analysis can be an effective non-invasive method to detect thyroid malignancies. Among the available thyroid nodule imaging methods, ultrasonography is cost-effective compared to other methods like Computed Tomography (CT) and Magnetic Resonance Imaging (MRI) [4]. Ultrasonographic imaging does not cause any health hazards unlike CT which uses harmful radiations. Benign and malignant thyroid nodules have distinguishable sonographic characteristics. Benign nodules have very little internal flow compared to that of malignant nodules [5]. Ultrasound images of the malignant nodule show the presence of a peripheral ring, while it can be present or absent in benign module [5]. However, a manual interpretation of these changes is subjective, and may result in low diagnostic accuracy. Moreover, speckle noise, which is a granular interference pattern, can also degrade the quality of ultrasound (US) images, thus making the diagnostic interpretation difficult. To address these limitations, in this work, we propose a Computer Aided Diagnostic (CAD) thyroid nodule characterization framework (named after our previous conceptual system – ThyroScan™) that incorporates (a) a Complex Wavelet Transform (CWT) step to reduce the speckle noise, (b) a feature extraction step that uses non-linear Higher Order Spectra (HOS) information to quantify the sonographic changes that manifest as textural changes in the image, and (c) a classification module that uses the texture features in classifiers to detect the presence or absence of malignancy.

High-Resolution Ultrasonography (HRUS) is a widely used method for diagnosing thyroid abnormalities [6] which has resolution high enough to reveal formations with size in the order of 1 mm. In our earlier work, we achieved 100% classification accuracy to detect thyroid malignancy using 3D HRUS images [7]. HRUS was chosen instead of CEUS due to the fact that overlapping findings in the

case of CEUS limited its potential in distinguishing malignant and benign thyroid lesions. In this paper, however, we overcome the limitation of CEUS images by processing it with an intermediate CWT stage. Moreover, the ultrasound contrast agent is not potentially nephrotoxic and so CEUS may be a first choice method for thyroid nodules diagnosis especially in patients of high risk of kidney failure [8]. Also, the contrast agent enhances the vasculature representation of the thyroid in CEUS images which is useful for distinguishing benign and thyroid nodules. Therefore, we were motivated to develop a reliable CAD system that works on CEUS images.

The objectives of this work are as follows: (1) to show the importance of processing CEUS ultrasound images to remove unwanted noise by introducing a CWT stage before features are extracted from the images; (2) to develop an automated system to accurately classify thyroid nodules to benign and malignant; and (3) to use our technique as a reliable adjunct protocol and thereby alleviate the need for the labor-intensive and invasive Fine Needle Aspiration (FNA) biopsy, which is currently the gold standard [9], in the early stages of disease management.

Our CAD system is represented in Figure 1. In the off-line training system, after the CWT stage, significant HOS features and ground truth of whether the image is benign or malignant are used to train a Fuzzy classifier. In the on-line system, the trained classifier is used to perform real-time classification of thyroid nodules into benign and malignant. We have thus combined CAD techniques with ultrasound image analysis [10] for objective analysis. We compared the performance of the classifier with and without the CWT stage. If CWT stage is not included, HOS features are directly extracted from the raw (i.e. unprocessed) CEUS images. We found that the inclusion of CWT stage resulted in tremendous improvement in the performance of the classifier in distinguishing malignant and benign thyroid nodules.

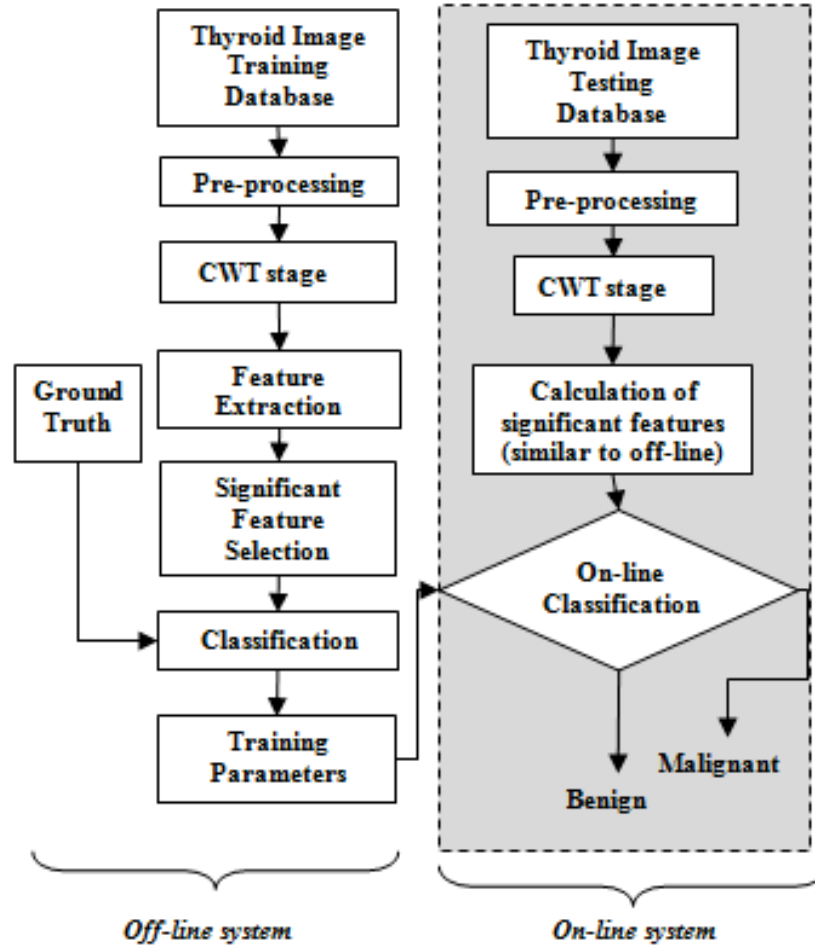


Figure 1. Block diagram of the proposed CAD technique for thyroid nodule characterization; The blocks outside the dotted shaded rectangular box represent the flow in the off-line training system, and the blocks within the dotted box indicate the on-line system.

### Patient selection

30 patients with the presence of goiter nodule (multi-nodule goiter cases excluded) were selected for the initial screening tests. A signed informed consent was obtained prior to image acquisition from patients and approval was also obtained from the ethical committee of the Endocrinology Section of the “Umberto I” Hospital of Torino in Italy. Accurate diagnosis of nodules was done using FNA biopsy and CEUS image examinations. We confirmed that the malignant images obtained had characteristics of malignancy like intra-nodular microcalcifications, hypoechoic appearance and irregular margins [11]. The

FNA examination produced the following diagnosis results for the 30 patients: five patients had benign goiter nodules which can be classified as THY2 (*Group1*:non-neoplastic). 25 patients had the characteristics of follicular neoplasm. They were classified under the group THY3 (*Group2*: follicular lesion/suspected follicular neoplasm) and were subjected to thyroidectomy. Among these 25 patients, five had nodule diameter exceeding 6 cm. Manual scanning is inadequate to capture such big lesions, and hence, these patients were excluded from the study. Three patients were excluded since they swallowed and coughed in between the CEUS test, producing motion artifacts in the recorded images. Two cases of concomitant thyroiditis were also eliminated. The shortlisted 15 *Group2* patients can be further grouped as follows: five benign (follicular neoplasm) cases and 10 malignant cases (seven papillary, one follicular neoplasm, two Hurtle cells carcinoma). Thus, including the earlier mentioned five benign goiter nodule patients (*Group1*), we had 10 benign patients and 10 malignant patients. Clinical examination and hormonal profiling were conducted for all the 20 patients. Among these 20 patients, 10 were males (age:  $53.5 \pm 13.3$  years; range: 22-71 years) and 10 females (age:  $50.1 \pm 10.8$  years; range: 25-68 years). The average size of benign/malignant nodules was  $31.7 \pm 17.9$  mm with range of 10-52 mm.

### **CEUS image acquisition and pre-processing**

For acquiring the CEUS images, 2.5 mL of Sonovue (an ultrasound contrast agent) was intravenously injected. It was so arranged that 50 seconds after the contrast agent was injected, a freehand scanning was performed for all the 20 patients by a trained expert who had more than 30 years of experience in neck ultrasonography. MyLab70 ultrasound scanner (Biosound-Esaote, Genova, Italy) equipped with a LA-522 linear probe that works in the range 4–10 MHz was used. In our work, images were acquired at 5 MHz with an average frame acquisition rate of 16 frames/second. The background average intensity was calibrated to be less than 5 in a 0-255 linear scale. The acquired 3D volumes were transferred to an external workstation in DICOM format for further processing and reconstruction. The following are the different stages employed for the processing of the acquired CEUS images:

- Pre-processing stage: all the 3D volume images were initially converted to double precision format.

Subsequently, attenuation of the intensity artifacts present in the images was done by applying a linear ramp with decreasing intensity from 1 to 0. This was followed by a normalization stage, a low pass filtering stage and then an initial speckle noise reduction (using a first order statistic filter) stage.

- Microbubble detection.
- **Threshold processing and 3D reconstruction.**

40 images were selected from each of the 10 patients with benign nodules and 10 patients with malignant nodules. Thus, 400 benign images and 400 malignant images were used to test the efficiency of the proposed system. Henceforth, we refer to these raw CEUS images of benign and malignant nodules as unprocessed (UNPR) images.


### **Image denoising and grayscale feature extraction**

The relevant characteristics of the CEUS images are captured by features. The mapping from images to features is a way of extracting objective information instead of using subjective information. We used CWT for speckle noise reduction and HOS based analysis methods to extract features.


#### *Image Denoising: Use of Complex Wavelet Transform (CWT) domain filter*

Several adaptive filters like Lee filter, Kaun filter, Frost filter, Sigma filter, and Gamma MAP filter have been used to reduce the speckle noise in US images [12]. But it has been observed that these filters lead to suppression of image features and useful information along with speckle noise, causing ambiguity in interpretation. **Recently, CWT has established an impressive reputation as a tool for image denoising as it gives much better directional selectivity while maintaining the low-redundancy [13, 14].** The unprocessed CEUS images (Figure 2(a) and Figure 2(b)) are passed through CWT filter for speckle noise reduction. The processed (PR) images are obtained from the output of the CWT filter (Figure 3(a) and Figure 3(b)).



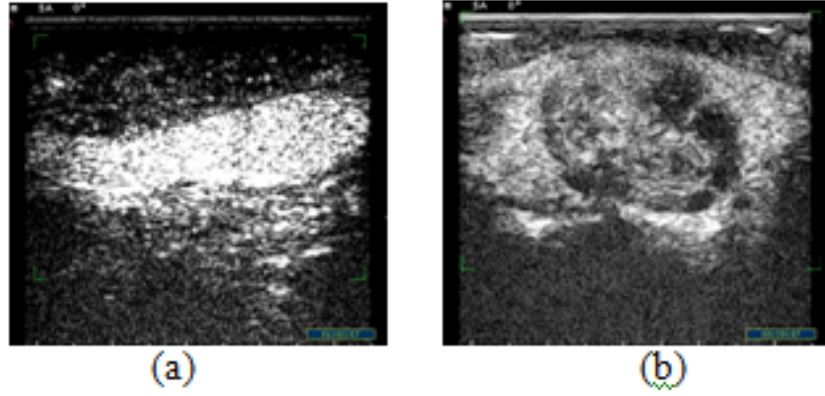

**Figure 2. Thyroid CEUS unprocessed images of (a) benign and (b) malignant cases.**

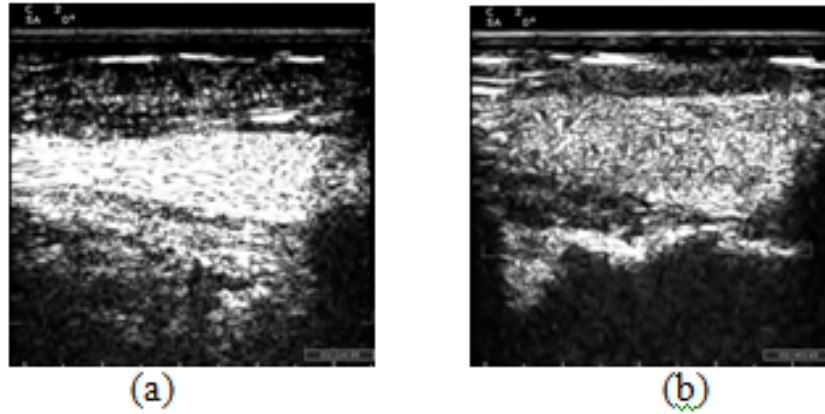

**Figure 3. Thyroid CEUS processed images of (a) benign and (b) malignant cases.**

In this work, the employed CWT filter uses the Generalized Nakagami Density (GND) function to approximate the speckle statistics under different scattering conditions commonly encountered in medical US images [15, 16]. Subsequently, a Bayesian threshold is derived to threshold the high-pass wavelet coefficients of the noisy image. This filter is scale and spatially adaptive as it adapts itself to the local image statistics and speckle statistics which vary from finer to coarser scales [17]. The CWT stage consists of mainly three steps. First, the image is decomposed into several scales through a multi-orientation analysis using two dimensional (2D) CWT. CWT uses filter banks to decompose signals into low and high pass components (represented by wavelet coefficients) called sub-bands. Low pass sub-

bands give information about slow varying signal characteristics, while high pass sub-bands are indicative of fast changes in the signal as well as noise. Next, the Bayesian thresholding is applied to process the noisy wavelet coefficients ( $Y$ ) of detail sub-bands [18] and finally, the de-noised image ( $X$ ) is synthesized from the processed (thresholded) wavelet coefficients through the inverse complex wavelet transform [19,20]. CWT decomposes an image  $f(t)$ ,  $t = (t_1, t_2) \in R^2$  using a complex scaling function and six complex wavelet functions as

$$f(t) = \sum_{b \in B} \sum_{j \geq j_0}^J \sum_{k=-\infty}^{\infty} D_f(j, k) \psi_{j,k}(t) + \sum_{k=-\infty}^{\infty} C_f(J, k) \phi_{J,k}(t) \quad (1)$$

where,  $\phi_{J,k}$  and  $\psi_{j,k}$  are complex;  $\phi_{J,k} = \phi_{J,k}^r + \sqrt{-1} \phi_{J,k}^i$ ,  $\psi_{j,k} = \psi_{j,k}^r + \sqrt{-1} \psi_{j,k}^i$ . The  $\psi_{j,k}^r$  and  $\psi_{j,k}^i$  are themselves real wavelets; where,  $D_f(j, k)$  and  $C_f(J, k)$  are the wavelet and scaling function coefficients respectively.  $J_0$  is an arbitrary starting scale for coarsest resolution and  $J$  is an arbitrary finite upper limit for highest resolution with  $J > J_0$ . The real and imaginary parts of the CWT are computed using separate filter bank structures with wavelet  $h_{0a}$ ,  $h_{1a}$  for the real part and  $h_{0b}$ ,  $h_{1b}$  for the imaginary part. The six sub bands of the 2D CWT are labeled as  $B = \{+15^0, +45^0, 75^0, -15^0, -45^0, -75^0\}$  for the six-oriented directions of the wavelet function. In CWT, complex coefficients of CWT are calculated using a dual tree of wavelet filters, each obtaining the real and imaginary magnitude parts [20]. The implementation of a filtering algorithm in CWT domain is very similar to the Discrete wavelet transform (DWT) domain. The principle difference is that the thresholding is applied to the magnitudes of the complex coefficients in order to achieve nearly shift-invariance as the small signal shifts may affect the real and imaginary parts keeping the overall magnitude same.

The implementation of the CWT domain-filtering algorithm is summarized as follows [21]:

1. Compute the CWT of the noisy image ( $f$ ).
2. Specify the value of tuning parameter ( $K$ ), which controls the degree of noise suppression.
3. Estimate the noise variance ( $\sigma^2$ ) using equation (2)

4. For each resolution scale,  $j$ ,  $1 \leq j \leq J$ , and

For each direction (negative and positive),  $D$ ,  $1 \leq D \leq 2$ ,

For each orientation,  $i \in \{HH_j^D, LH_j^D, HL_j^D\}$

For all the spatial locations,  $l = 1, 2, \dots, M$

Compute the standard deviation,  $\sigma_X$ , using equations (3), (4) and (6).

If  $\sigma_X > 0$ , estimate the coefficient,  $\hat{x}_l$ , using equation (5), otherwise set  $\hat{x}_l = 0$

5. Apply the inverse CWT to get the denoised image ( $g$ )

$$\hat{\sigma}^2 = \left[ K \frac{\text{median}(|Y_l|)}{0.6745} \right]^2 \quad Y_l \in \{HH_1, HH_2\} \quad (2)$$

$$\sigma_y^2 = \sigma_x^2 + \Omega; \quad (3)$$

$$\hat{\sigma}_x^2 = \max(\hat{\sigma}_y^2 - \Omega, 0) \quad (4)$$

$$\hat{x} = \text{sign}(y) \left( \max \left( 0, \frac{2s|y|}{B} - \frac{\Omega + \sqrt{\Omega^2 - 8As(s-1)(Ay^2 - \sqrt{2}\Omega y) + 2ABC}}{\sqrt{2AB}} \right) \right) \quad (5)$$

$$\Omega = (K_1 \sigma^2)^s \quad \text{and} \quad K_1 = \frac{m^{1/s} \cdot \Gamma(m)}{\Gamma(m+1/s)} \quad (6)$$

where,  $A = ms\sigma_x y^{2s-2}$ ,  $B = 2s(2s-1)$ , and  $C = (2ms-1)\Omega\sigma_x$ .  $m$  and  $s$  are the shape adjustment parameters of generalized Nakagami distribution. The shrinkage function given in equation (5) named as *GNDThresh* can be easily deployed to derive the thresholding estimators for the density functions belonging to the generalized Nakagami family [21].


*Grayscale feature extraction: Higher Order Spectra (HOS)*

Before the HOS parameters are evaluated, the pre-processed and complex wavelet transformed US

images were subjected to Radon transform [22]. The Radon transform rotates the image around its centre through different angles  $\theta$  and then computes line integrals along many parallel paths in the image, transforming the intensity along these lines into points of the resultant signal. Thus, the input for the Radon transform is an image and the output is a one-dimensional signal at various angles. From the one-dimensional signal, HOS parameters are extracted at a constant angle interval of  $45^\circ$  (at  $0^\circ, 45^\circ, 90^\circ, 135^\circ, 180^\circ$ ). HOS (Polyspectra) is the spectral representation of higher order statistics, i.e. moments and cumulants of third and higher order which can be used for deterministic signals and random processes. Since the HOS of Gaussian signals are statistically zero, it can measure non-Gaussianity and offers good noise immunity. HOS can preserve the true phase information of signals and can detect nonlinearity. HOS features used in this study are derived from the bispectrum. Bispectrum  $B(f_1, f_2)$  is the third order statistics of the signal given by

$$B(f_1, f_2) = E[X(f_1)X(f_2)X(f_1 + f_2)] \quad (7)$$

where  $X(f)$  is the Fourier transform of the signal  $x(nT)$ ,  $n$  is an integer index,  $T$  is the sampling interval and  $E(\cdot)$  is expectation operator. The frequency  $f$  may be normalized by the Nyquist frequency (half of the sampling frequency) for values to lie between 0 and 1. The region  $\Omega$  of computation of bispectrum and bispectral features of a real signal is uniquely given by a triangle  $0 \leq f_2 \leq f_1 \leq f_1 + f_2 \leq 1$  as given in Figure 4.

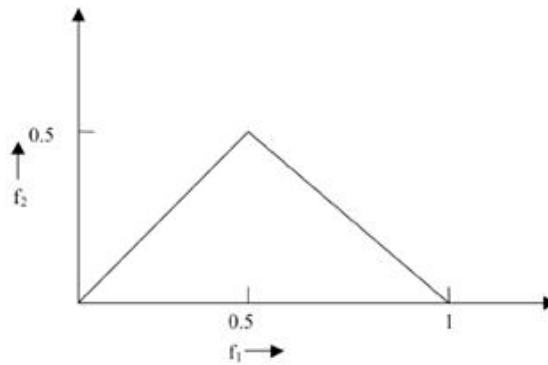

**Figure 4. Principal domain or non-redundant region  $\Omega$  of computation of the bispectrum for real signals. Frequencies are shown normalized by the Nyquist frequency.**

We determined the mean of magnitude as follows

$$m\text{Amp} = \frac{1}{L} \sum_{\Omega} |B(f_1, f_2)| \quad (8)$$

The following  $H$  parameters, which are related to the moments of bispectrum, were also calculated in this work. The sum of logarithmic amplitudes of bispectrum  $H_1$  is given by

$$H_1 = \sum_{\Omega} \log(|B(f_1, f_2)|) \quad (9)$$

The sum of logarithmic amplitudes of diagonal elements in the bispectrum  $H_2$  is given by

$$H_2 = \sum_{\Omega} \log(|B(f_k, f_k)|) \quad (10)$$

The first order spectral moment of amplitudes of diagonal elements of the bispectrum  $H_3$  is

$$H_3 = \sum_{k=1}^N k \log(|B(f_k, f_k)|) \quad (11)$$

$$H_4 = \sum_{k=1}^N (k - H_3)^2 \log(|B(f_k, f_k)|) \quad (12)$$

All the above features are defined over a principal domain  $\Omega$ .  $L$  is the number of points within the region  $\Omega$ . More details of equations for the HOS features  $m\text{Amp}$ ,  $H_1$ ,  $H_2$ ,  $H_3$  and  $H_4$  are given in [23].

### Feature selection

We used Student's  $t$ -test to study if the mean value of a feature is significantly different between the benign and malignant groups. The result of the  $t$ -test is the  $p$ -value, which is compared with a level of significance ( $\alpha$ -level). Popular levels of significance are 5% (0.05), 1% (0.01) and 0.1% (0.001). If the  $p$ -value is lower than the  $\alpha$ -level, it indicates that the feature is powerful enough to be different for the two classes. In this work, we chose  $\alpha$ -level as 0.001, and observed that the features had  $p$ -values even lower than 0.0001 indicating their strength as valuable discriminators of the two classes.

### Classification

We chose the Fuzzy classifier for developing the data mining framework as Fuzzy classifier is a rule-based classifier which is more comprehensible to the end-user. We used a subtractive clustering technique using the Sugeno technique [24] to generate a Fuzzy Inference System (FIS) [25]. FIS contains set of fuzzy rules which are used to perform fuzzy inference calculations to obtain the class label of the test data. We used ten-fold stratified cross validation data resampling technique to train and test the classifiers. 800 data sets belonging to benign and malignant classes were split into ten parts randomly, such that each part had the same proportion of images from both classes. During the training phase, nine parts containing 720 images (320 benign and 320 malignant) with the corresponding class label were used to train the classifier and to obtain the classifier parameters. During the test phase, the trained classifiers were used to predict the class of the remaining part (80 samples) of the dataset and to calculate the performance measures. This process was repeated nine more times using different test sets. Then, the average of the performance measures obtained for each of the ten folds was calculated. The efficiency of the classifier to properly classify the images into their correct classes is given by the performance evaluation parameters namely sensitivity, specificity, Positive Predictive Value (PPV), and accuracy. High values for the evaluation parameters indicate high classifier performance.

## Results

### *Significant HOS features*

Table 1 and 2 show the significant HOS features ( $p$ -value  $< 0.0001$ ) obtained from the processed images (on which CWT was used for speckle noise reduction) and the unprocessed (no CWT stage) CEUS images, respectively, for the  $90^\circ$  Radon Transform angle. HOS parameters were obtained at an interval of  $45^\circ$  in the range of  $0^\circ$ - $180^\circ$ . We observed that in both the CEUS processed and unprocessed data sets, the values of the significant features ( $mAmp$ ,  $H_1$ ,  $H_2$ ,  $H_3$ , and  $H_4$ ) remained the same for all the angular measurements. Thus, the significant HOS parameters obtained are unique irrespective of the angle of measurement. All the five HOS parameters were observed to be low for benign compared to malignant group. Therefore, for training the classifiers, we used only the five significant features obtained using the

90° angle in both processed and unprocessed cases. The use of this reduced significant feature set makes the design and training of the classifier simpler and faster.

**Table 1.** Range (mean  $\pm$  standard deviation) of the significant features that had a  $p$ -value less than 0.0001 for CEUS processed images

Feature (90° angle)	Benign	Malignant
$mAmp$	2.557E+15 $\pm$ 2.475E+15	4.651E+15 $\pm$ 2.353E+15
$H_1$	5.450E+04 $\pm$ 1.349E+03	5.570E+04 $\pm$ 984
$H_2$	891 $\pm$ 19.0	912. $\pm$ 13.6
$H_3$	2.809E+04 $\pm$ 657	2.874E+04 $\pm$ 461
$H_4$	7.023E+11 $\pm$ 4.798E+10	7.525E+11 $\pm$ 3.507E+10

**Table 2.** Range (mean  $\pm$  standard deviation) of the significant features that had a  $p$ -value less than 0.0001 for CEUS unprocessed images

Feature (90° angle)	Benign	Malignant
$mAmp$	3.38 $\pm$ 0.128	3.47 $\pm$ 7.160E-02
$H_1$	5.901E+04 $\pm$ 995	6.020E+04 $\pm$ 846
$H_2$	967 $\pm$ 13.6	990 $\pm$ 12.1
$H_3$	3.068E+04 $\pm$ 461	3.135E+04 $\pm$ 376
$H_4$	9.095E+11 $\pm$ 4.018E+10	9.720E+11 $\pm$ 3.501E+10

### *Classification results*

The parameters of accuracy, PPV, sensitivity and specificity were determined using the CEUS generated thyroid images with and without using CWT stage for speckle noise reduction. The results of the classification are shown in Table 3. All the four performance measures had marked improvement in the

case of the processed images compared to the unprocessed images. We observed that on using the Fuzzy classifier on the processed CEUS images, the accuracy went up to 99.1% from the 91.6% which was obtained using the unprocessed images. The other parameters also showed similar increase.

**Table 3.** Performance measures of the classifiers (A: accuracy; Sn: sensitivity; Sp: specificity) (all values in %) (UNPR: unprocessed; PR: processed)

Classifier	UNPR				PR			
	A	PPV	Sn	Sp	A	PPV	Sn	Sp
Fuzzy	91.6	91.2	93.8	91.6	99.1	98.6	99.8	98.5

## Discussion

### *Literature review*

FNA biopsy has the limitation of the need for an expert physician to conduct the test. When combined with carefully chosen parameter extraction methods and CAD based techniques, ultrasound imaging, which is non-invasive and affordable, has emerged as a comparable contender to FNA to differentiate benign and malignant thyroid nodules. It is sensitive enough to serve as a predictor to thyroid malignancy [11]. In ultrasound image processing, useful features are extracted to study the image texture differences and echographic patterns to identify the presence of abnormalities in thyroid nodule. In CEUS, malignancy is indicated by the presence of heterogeneous enhancement, while ring enhancement is prominent in benign nodules [26]. Many works have been conducted for automated benign-malignant thyroid nodule characterization. These studies have used techniques such as molecular profiling [27], genetic markers [28], elastography [29], and fluorescent scanning [30] for thyroid nodule classification. Though the objective of all these works is the same, they differ in input data format, features extracted, methods and classifiers used and in classification efficiency.

In the case of ultrasound based studies, color and power Doppler imaging were already ruled out as they were not suitable for 3D microvessel detection due to undesirable color blooming in high perfusion



cases and poor spatial resolution. In one study [31], the accuracy of quantitative analysis of tumor vascularity on power Doppler sonograms was analyzed, and using vascular indices, an accuracy of only 84.5% was reached. The most significant characteristic of malignant thyroid nodule is the extensive internal flow. CEUS, with intravenously administered contrast agent, can represent micro and macrovasculature and the internal flow of thyroid nodules much effectively compared to HRUS. Molinari *et al.* [32] quantified seven vascular parameters like vascular density, number of branching nodes etc. for 3D CEUS benign and malignant images, but did not use them for classification. Therefore, in 2011, our team worked on developing data mining strategies that use significant features from HRUS and CEUS images for thyroid nodule characterization and classification. In one study [7], we used 3D HRUS data set to obtain five features out of which three were texture features and two were Discrete Wavelet Transform (DWT) features and used them in an AdaBoost classifier with perceptron as weak learner to achieve 100% accuracy, sensitivity and specificity. In another recent study [33], we extracted ten significant features (three texture features and seven DWT features) from 3D CEUS thyroid images to obtain an accuracy of 98.9%, sensitivity of 98% and specificity of 99.8% using KNN classifier. Thus, even though HRUS image analysis has reached its perfection in terms of classifier performance [7], we observed that there is still scope for improvement of detection accuracy using CEUS images [33]. These were the reasons behind choosing CEUS data for this study.

#### *Key features of this study*

In this study, we used Sonovue which is a microbubble-based contrast agent that does not come out of the vessel lumen. Any echo received from a microbubble is an indication of the presence of a vessel [34]. Hence, CEUS with Sonovue will give a better depiction of vascularity. We have included CWT to process CEUS images before the extraction of HOS features to deal with speckle noise. Our proposed technique has the following features:

- Ultrasonography, in addition to being affordable and non-invasive, is highly effective and safe. It can detect thyroid nodules as small as 3 mm [35]. Ultrasound waves are not known to cause any health hazards, they are absolutely safe.

- We used 3D imaging instead of 2D, so that the feature of nodule volume can also be utilized for diagnosis.
- The CEUS data acquisition method is low cost and the proposed automation system consists of algorithms implemented in software which are also affordable.
- The CWT stage suppresses the disturbances in US images like echo perturbations and speckle noise and preserves features better than DWT. It is especially useful in CEUS images which contain strong diagonal features as CWT preserves features oriented at angles  $45^\circ$  and  $-45^\circ$  without combining them. Ours is the only work which includes CWT for processing of US images. Due to good shift-invariance (as the shrinkage rule is applied to the magnitude of each of the complex coefficients) and good directional-sensitivity of CWT, our CEUS image filtering techniques yielded better performance than the earlier DWT based methods.
- Computational complexity of CWT is low, making it suitable for on-line real time applications.
- We have validated our speckle reduction results (obtained after CWT stage) both qualitatively (from two radiologist) and quantitatively in terms of various image quality parameters like CNR, SNR and Edge preservation Index [21]. Detailed results are submitted in a paper which is under review. Further, the efficiency of CWT stage is cross-validated by the classifier which results in 99.1% accuracy.
- We avoided the common problem of classifier over-fitting by adopting ten-fold cross validation technique for data resampling.
- The number of significant features to be given as input to the classifier to obtain very high accuracy is very less (just five features) for processed as well as unprocessed CEUS images. This makes the design and training of the classifier simpler.
- The Fuzzy classifier resulted in the highest accuracy of 99.1% for the processed images, which is higher than previously published results.
- Instead of using the commonly used vascular and texture features, we have, in this work, exploited the capability of popular nonlinear dynamics theory based HOS features to classify thyroid lesions and

achieved the maximum possible accuracy.

## Conclusions

Thyroid malignancy analysis using ultrasonography is a non-invasive, affordable and safe diagnostic test which produces images depicting the prominent structure and features of thyroid nodule. We have investigated the implication of introducing CWT stage for speckle noise reduction before HOS features are extracted from CEUS images. We have demonstrated that the initial processing of CEUS images with CWT stage significantly improves the efficiency of the automated real-time system in characterizing the thyroid nodules into benign and malignant classes. The Fuzzy classifier resulted in the highest accuracy of 99.1% for the CWT processed images, sensitivity of 99.8%, specificity of 98.5%, and PPV of 98.6%.

## References

1. Lansford CD and Teknos TN. Evaluation of the Thyroid Nodule. *Cancer Control* 2006; 13:89-98.
2. ACS (American Cancer Society) What are the key statistics about thyroid cancer? Available: <http://www.cancer.org/Cancer/ThyroidCancer/DetailedGuide/thyroid-cancer-key-statistics>
3. NCI (National Cancer Institute) on thyroid cancer. Available: <http://www.cancer.gov/cancertopics/types/thyroid>.
4. Soto GD, Halperin I, Squarcia M, et al. Update in thyroid imaging. The expanding world of thyroid imaging and its translation to clinical practice. *Hormones (Athens)* 2010; 9: 287-298.
5. Ivanac G, Brkljacic B, Ivanac K, et al. Vascularization of benign and malignant thyroid nodules: CD US evaluation. *Ultraschall Med* 2007; 28: 502-506.
6. Polyzos SA, Kita M, Avramidis A. Thyroid nodules - stepwise diagnosis and management. *Hormones (Athens)* 2007; 6:101-119.
7. Acharya UR, Faust O, Sree SV, et al. ThyroScreen System: High Resolution Ultrasound Thyroid image characterization into benign and malignant classes using novel combination of texture and discrete wavelet transform. *Comput Methods Programs Biomed* 2012; 107: 233-241.

8. Claudon M, Cosgrove D, Albrecht T, et al. Guidelines and good clinical practice recommendations for contrast enhanced ultrasound (CEUS) - update 2008. *Ultraschall Med* 2008; 29:28-44.
9. Baloch ZW, Fleisher S, LiVolsi VA et al. Diagnosis of follicular neoplasm: a gray zone in thyroid fine-needle aspiration cytology. *Diagn Cytopathol* 2002; 26:41-44.
10. Suri JS, Kathuria C and Molinari F. *Atherosclerosis Disease Management*. New York: Springer, 2011.
11. Bastin S, Bolland MJ and Croxson MS. Role of ultrasound in the assessment of nodular thyroid disease. *J Med Imaging Radiat Oncol* 2009; 53:177-187.
12. Gupta S, Chauhan RC and Saxena SC. Homomorphic wavelet thresholding technique for denoising medical ultrasound images. *J Med Eng Technol* 2005; 29:208-214.
13. Kingsbury N. The dual tree complex wavelet transform: a new technique for shift invariance and directional filters. *Proceedings of 8th IEEE DSP Workshop*, Bryce Canyon, 1998.
14. Dudy A, Singh K. A new approach for denoising Ultrasonographic Images using DTCWT. *Int J Latest Res Sci Technol* 2012; 1:106-108.
15. Shankar PM. Ultrasonic tissue characterization using a generalized Nakagami model. *IEEE Trans Ultrason Ferroelectrics Freq Contr* 2001; 48: 1716-1720.
16. Gupta S, Chauhan RC and Saxena SC. Robust non-homomorphic approach for speckle reduction in medical ultrasound images. *Med Biol Eng Comput* 2005; 43:189-195.
17. Pizurica A, Philips W, Lemahieu I, et al. A versatile wavelet domain noise filtration technique for medical imaging. *IEEE Trans Med Imaging* 2003; 22:323-331.
18. Jansen M. *Noise reduction by wavelet thresholding*. Springer Verlag, Lecture notes in Statistics 2001; p.161.
19. Gupta S, Kaur L, Chauhan RC, et al. A wavelet based statistical approach for speckle reduction in medical ultrasound images. *IEEE proceedings, TENCON* 2003; 2: 534-7.
20. Achim A, Bezerianos A, Tsakalides P. Novel Bayesian multiscale method for speckle removal in medical ultrasound images. *IEEE Trans Med Imaging* 2001; 20; 772-783.

21. Gupta S, Chauhan RC, Saxena SC. A versatile technique for visual enhancement of medical ultrasound images,” *Digital Signal Processin* 2007; 17: 542-556.
22. Ramm A, Katsevich A. *The radon transform and local tomography*. CRC Press, 1996.
23. Chua KC, Chandran V, Acharya UR, et al. Application of higher order statistics/spectra in biomedical signals - A review. *Med Eng Phys* 2010; 32:679-689.
24. Sugeno M. *Industrial applications of fuzzy control*. Elsevier Science Pub. Co., 1985.
25. Ross TJ. *Fuzzy logic with engineering applications*. West Sussex, UK: John Wiley & Sons Ltd, 2004.
26. Zhang B, Jiang YX, Liu JB, et al. Utility of contrast-enhanced ultrasound for evaluation of thyroid nodules. *Thyroid* 2010; 20:51-57.
27. Finley DJ, Zhu B, Barden CB, et al. Discrimination of benign and malignant thyroid nodules by molecular profiling. *Ann Surg* 2004; 240:425-436.
28. Cerutti JM, Delcelo R, Amadei MJ, et al. A preoperative diagnostic test that distinguishes benign from malignant thyroid carcinoma based on gene expression. *J Clin Invest* 2004; 113:1234-1242.
29. Hong Y, Liu X, Li Z, et al. Real-time ultrasound elastography in the differential diagnosis of benign and malignant thyroid nodules. *J Ultrasound Med* 2009; 28:861-867.
30. Patton JA, Hollifield JW, Brill AB, et al. Differentiation between malignant and benign solitary thyroid nodules by fluorescent scanning. *J Nucl Med* 1976; 17:17-21.
31. Lyshchik A, Moses R, Barnes SL, et al. Quantitative analysis of tumor vascularity in benign and malignant solid thyroid nodules. *J Ultrasound Med* 2007; 26:837-846.
32. Molinari F, Mantovani A, Deandrea M, et al. Characterization of single thyroid nodules by contrast-enhanced 3-D ultrasound. *Ultrasound Med Biol* 2010; 36: 1616-1625.
33. Acharya UR, Faust O, Sree SV, et al. Cost-effective and non-invasive automated benign and malignant thyroid lesion classification in 3D contrast-enhanced ultrasound using combination of wavelets and textures: a class of ThyroScan™ algorithms. *Technol Cancer Res Treat* 2011; 10:371-380.

34. Schneider M, Arditi M, Barrau MB, et al. BRI: a new ultrasonographic contrast agent based on sulfur hexafluoride-filled microbubbles. *Invest Radiol* 1995; 30:451-457
35. Mandel SJ. Diagnostic use of ultrasonography in patients with nodular thyroid disease. *Endocr Pract* 2004; 10: 246-252.