

Assessment of Preload Loss after Cyclic Loading in the OT Bridge System in an “All-on-Four”
Rehabilitation Model in the Absence of One and Two Prosthesis Screws

Original

Assessment of Preload Loss after Cyclic Loading in the OT Bridge System in an “All-on-Four” Rehabilitation Model in the Absence of One and Two Prosthesis Screws / Pozzan, M.C., Grande, F., Mochi Zamperoli, E., Tesini, F., Carossa, M., Catapano, S.. - In: MATERIALS. - ISSN 1996-1944. - 15:4(2022), p. 1582. [10.3390/ma15041582]

Availability:

This version is available at: 11583/2973721 since: 2022-12-09T14:57:31Z

Publisher:

MDPI

Published

DOI:10.3390/ma15041582

Terms of use:

This article is made available under terms and conditions as specified in the corresponding bibliographic description in the repository

Publisher copyright

(Article begins on next page)

Article

Assessment of Preload Loss after Cyclic Loading in the OT Bridge System in an “All-on-Four” Rehabilitation Model in the Absence of One and Two Prosthesis Screws

Mario Cesare Pozzan¹, Francesco Grande^{1,2,*} , Edoardo Mochi Zamperoli¹, Fabio Tesini¹, Massimo Carossa²  and Santo Catapano¹ 

¹ Department of Prosthodontics, University of Ferrara, Via Luigi Borsari 46, 44121 Ferrara, Italy; mariocesare.pozzan@edu.unife.it (M.C.P.); mochizamperolie@gmail.com (E.M.Z.); fabio.tesini@edu.unife.it (F.T.); cts@unife.it (S.C.)

² Department of Surgical Sciences CIR Dental School, University of Turin, Via Nizza 230, 10126 Turin, Italy; massimo.carossa@unito.it

* Correspondence: francesco.grande@unife.it; Tel.: +39-05-3268-8501

Abstract: The aim of this study was to evaluate the stability of prosthetic screws after applying cyclic loadings in an “all-on-four” rehabilitation model with the OT Bridge system. The model was tested both with and without anterior screws. Four implant analogues following the “all-on-four” concept were inserted in an edentulous mandibular resin model. An OT Bridge system with a Cr–Co prosthetic framework was fabricated. Depending on the presence or absence of one or two anterior screws on the implant analogues, three groups were created, i.e., Gr.1: three tightening screws, Gr.2: two tightening screws, Control Group: four tightening screws. Each single group underwent subsequent 400,000 cyclic loads, simulating approximately a year of chewing by using a dynamometer machine. This cycle was repeated five times for each group, and preload loss values were evaluated on each prosthetic screw after each cycle. All the data obtained were analyzed by one-way ANOVA and Student’s *t*-test. No statistically significant differences after intragroup analysis were found. A statistically significant difference within the Gr.1 between the screws in positions 33 and 36, equal to 15.2% (p -value = 0.0176), was found. The OT Bridge seems a useful system to maintain the retention of a prosthesis during mechanical stress conditions even in the absence of one screw in an “all-on-four” rehabilitation. This could represent a good solution to solve the esthetic problem of the screw buccal access hole for fixed solutions.

Keywords: preload loss; OT bridge; prosthetic connection; implant-supported prosthesis; loosening torque; all-on-four



Citation: Pozzan, M.C.; Grande, F.; Mochi Zamperoli, E.; Tesini, F.; Carossa, M.; Catapano, S. Assessment of Preload Loss after Cyclic Loading in the OT Bridge System in an “All-on-Four” Rehabilitation Model in the Absence of One and Two Prosthesis Screws. *Materials* **2022**, *15*, 1582. <https://doi.org/10.3390/ma15041582>

Academic Editor: Daniele Botticelli

Received: 19 January 2022

Accepted: 18 February 2022

Published: 20 February 2022

Publisher’s Note: MDPI stays neutral with regard to jurisdictional claims in published maps and institutional affiliations.



Copyright: © 2022 by the authors. Licensee MDPI, Basel, Switzerland. This article is an open access article distributed under the terms and conditions of the Creative Commons Attribution (CC BY) license (<https://creativecommons.org/licenses/by/4.0/>).

1. Introduction

One of the fixed solutions that has been commonly used for several years in implant prosthodontics for the complete-arch rehabilitation of the upper and lower jaws is the “all-on-four” protocol [1–3]. This technique consists in the insertion in the mandibular ridge of two anterior intra-foraminal implants perpendicular to the occlusal plane and two posterior angulated implants emerging in the second premolar/first molar position [4]. For the upper jaw, the position could be the same with respect to the anatomy of the maxillary sinuses. In this way, the “all-on-four” allows a complete arch rehabilitation using a fixed solution with only four implants, achieving a favorable implant distance with a short cantilever [5]. The most frequent complication, described in the literature for screw-in systems, is the loss of preload that is defined as the force established between the screw turns and the abutment thread [6,7]. Many factors could influence the loss of preload, which is a prodromal manifestation of the connecting screw fracture [8–10]. The relationship between preload and tightening torque (force exerted to tighten a screw)

depends on several factors: the type of implant–prosthetic connection, the morphology and material of the abutment, the design and material of the screw, tolerances between screw and thread, the morphology of the implant fixture, the type of prosthetic rehabilitation, iatrogenic errors [10,11].

In order to connect implants with prosthetic frameworks, the most used solution is today represented by the Multi Unit Abutment (M.U.A) which has the function to change the implant connection from an internal hexagon to an external one. When tilted implants are inserted to correct the implant axis and to solidarize distal implants with the anterior ones, angulated M.U.A components are necessary. In this system, the prosthetic screw is the only component that allows the binding between the prosthetic framework and the implants [12–15].

Recently, another screw-retained system, called OT Bridge[®] (Rhein 83 srl, Bologna, Italy), has been introduced on the dental market as an alternative to M.U.A. [16]. The OT Bridge is composed of a low-profile attachment for overdenture, the OT Equator, a sub-equatorial component represented by an interchangeable acetal ring called Seeger, and a cylindrical titanium “extragrade” abutment. This abutment is cemented in the prosthetic framework and, at its retentive extremity, is provided of a cavity designed for the insertion of the acetal ring which occupies the undercut created, allowing a first retention of the prosthesis with the OT Equator. In this way, the Seeger ring provides a secure and functioning elastic retention system that guarantees the stable housing of the prosthesis on the OT equator attachment even in the absence of the prosthetic screw which has a diameter of 1.6 mm.

An important clinical issue, arising with “screw-retained” rehabilitations, especially in the case of severely resorbed jaws, is the presence of a buccal screw access channel that constitutes an anesthetic problem independently of the prosthetic material use [17–21]. This issue could be managed with a “cemented-retained” solution, although the advantages of the screw-retained prosthesis are lost. Another way to solve this problem could be using angulated M.U.A abutment only for less than a 30° disparallelism [22]. In OT Bridge rehabilitations, this esthetic problem is maintained or amplified because the OT Equator follows the implant axis.

A possible solution, retaining the benefits of a screw-in prosthesis, may be provided by the OT-Bridge system [16] in the absence of one or two anterior prosthetic screws [23,24]. In this way, the stability of the OT Bridge system is provided by both the posterior screws and the interlocking system between the acetal Seeger, inserted in the extragrade abutment, and the subequatorial region of the OT equator attachments in the anterior region. However, it is not clear and there are no data available in the literature about the stability of this system during and after cyclic loadings without one or two screws.

Therefore, the aim of this study was to evaluate, in an “all-on-four” model with an OT Bridge prosthetic system, the stability of its connecting screws after cyclic loadings, both in the presence and in the absence of the anterior screws. The null hypotheses (H0) considered for this study were the absence of removal torque difference between the model without one or two screws and the model with all four screws (intergroups analysis—H0 nr.1) and the absence of removal torque difference between the values of the screws within each aforesaid solution (intragroup analysis—H0 nr.2).

2. Materials and Methods

2.1. Samples Preparation

A resin model, already described in a previous article [16], was fabricated (Figure 1a,b). Four implant analogues (3.5 × 10 mm; NobelBiocare, Kloten, Switzerland) with internal hexagonal connections were placed in intraforaminal position following the “all-on-four” concept [4]. Each implant was placed according to a predetermined angulation: the axes of implants in canine/lateral incisor position were orthogonal to the occlusal plan, while those of implants in second premolar/first molar area were distally tilted by 30°. A calibrated

hole was performed in the center of the model to fix it to the machine for the dynamometric control of the loads.

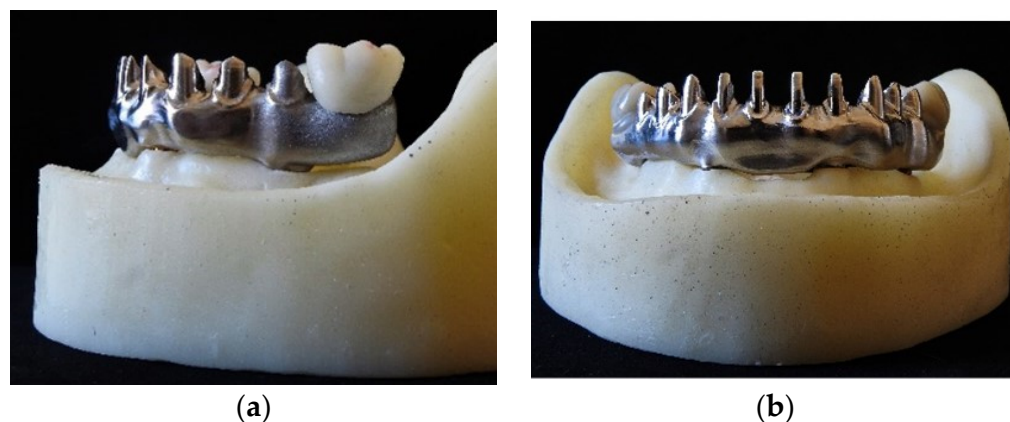


Figure 1. Lateral (a) and frontal views (b) of the model used.

A milled cobalt–chrome framework for hybrid prosthesis connecting the four implant analogues was fabricated from a digital STL file. Extragrade-titanium angulated and straight abutments (Rhein 83, Bologna, Italy) were used for the model.

According to the most predicted protocols described in the literature, two monolithic zirconia crowns, whose central fossa was 7 mm distal to the last implant analogue emergences (36 and 46), were distally positioned and cemented on the cobalt–chrome framework using the dual resinous cement OT Cem (Rhein83, Bologna, Italy) [25,26]. The cementation phase included the insertion of the crown on the appropriate housing and, to optimize the fit between the crown and the framework, the placement of a load of 10 N for 5 min through MTS Acumen (MTS Systems S.R.L, Turin, Italy) [27]. The load was then applied on the cemented monolithic zirconia crowns.

According to the indications proposed by the manufacturer (Rhein83, Bologna, Italy), the connection screws were tightened at 25 Ncm by means of the torque-controlled dynamometric micromotor Implant-Med-Plus (W&H, Brusaporto—BG, Italy); for this study, the white acetalic Seeger (standard seal) was used. After 10 min, a second screwing was performed at 25 Ncm, according to the screwing protocol proposed by Winkler et al. [28].

Depending on the presence or absence of one or two anterior screws on the implant analogues, three groups of five screws for removal torque evaluation after cyclic loadings were created and compared to each other (Figure 2):

1. Group 1 (Gr.1): Group with 3 tightening screws (33, 36, 46) inserted on 4 implant analogs without the screw in position 43.
2. Group 2 (Gr.2): Group with 2 tightening screws (36, 46) inserted on 4 implant analogs without the anterior screws 33 and 43.
3. Control Group (Gr.CTR): Group with 4 tightening screws (33, 43, 36, 46 inserted) on 4 implant analogs. This group was the same as that a previous study by Catapano et al. [16].

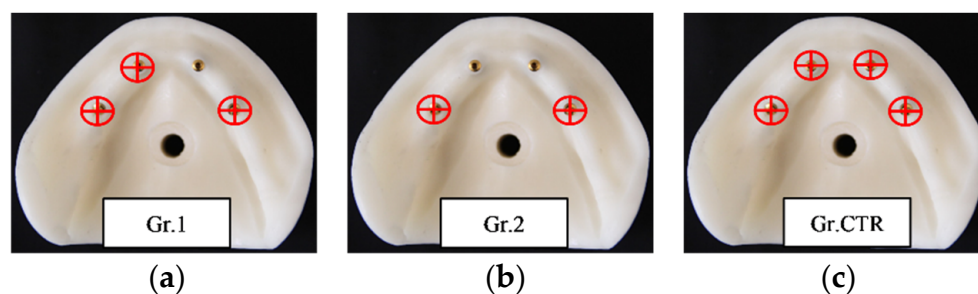


Figure 2. Representative images of the screws' placement in the three different groups. From the left to the right: Gr.1 (a), Gr.2 (b), and Gr.CTR (c).

2.2. Cyclic Test

The MTS Acumen, which is a dynamometer machine, was used to approximately simulate the developed effort of a year of chewing loads [29,30]. Each loading test consisted of 400,000 subsequent cycles with a variable force from 40 N to 400 N at the frequency of 1.6 Hz, orthogonally to the occlusal plane. The vertical excursion of the piston was 0.16 mm. (Figure 3). This cycle was repeated five times for each group.

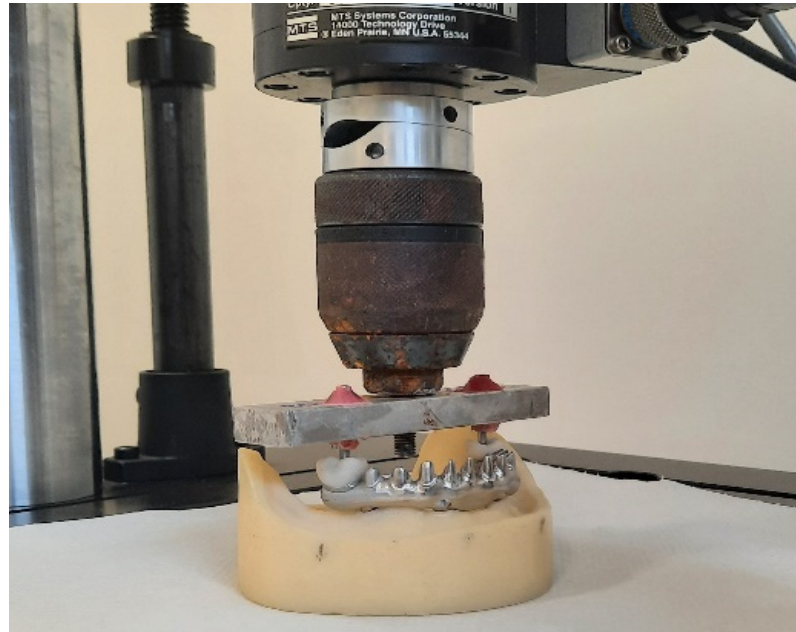


Figure 3. Representative image of the model placement under the MTS Acumen.

To simulate the oral cavity environment during cyclic load, the model was placed in a thermostatic water bath at a constant temperature of 37 °C. (Figure 4). To evaluate preload loss values, after each single cyclic load, the registration of the connection screw torque removal was performed using Implant-Med-Plus® on each tightening screw. After each single unscrewing session, the implant–prosthetic connection screws and the acetalic Seegers inserted in the cobalt–chrome framework were changed.

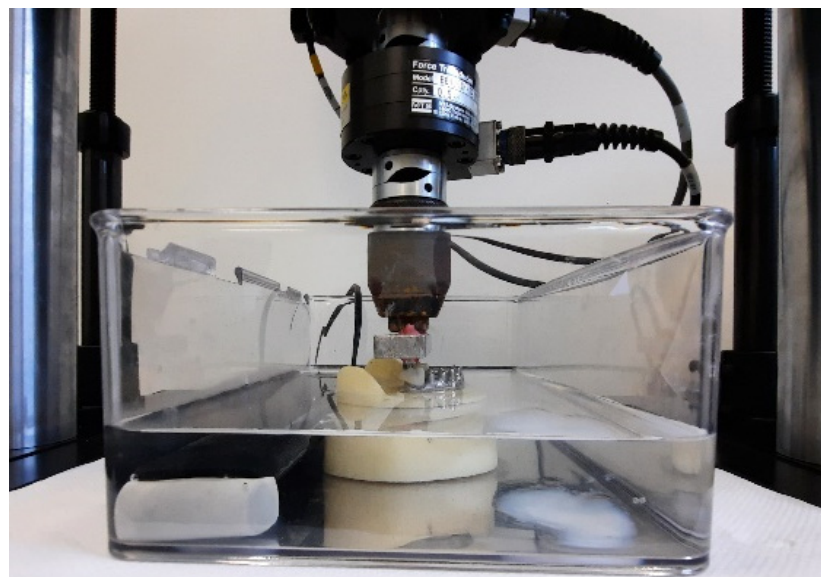


Figure 4. Image of the model during a cyclic load in the water bath.

2.3. Statistical Analysis

All the data obtained in this in vitro study were analyzed by statistical evaluations, which were carried out through the GraphPad Prism data analysis program® 9.2.0 and through statistical tests for variance, i.e., one-way ANOVA and Student’s *t*-test.

For both tests, the statistical significance was set at 0.05 (*p*-value < 0.05).

Using one-way ANOVA with Bonferroni correction, the following data were evaluated:

- differences between the averages mean values of preload loss for Gr.1, Gr.2, and Gr.CTR;
- differences in preload loss percentage values of the screws in positions 36 and 46 between the three different groups;
- differences in preload loss percentage values of the screws inside each group;

The following statistical analyses were performed using Student’s *t*-test:

- differences in percentage torque loss of screws positioned in zone 33 for Gr.1 and Gr.CTR.
- differences in percentage torque loss between the screws positioned in zones 36 and 46 in Gr.2.

The null hypotheses considered were:

- absence of removal torque difference between the three groups (intergroups analysis—H0 nr.1);
- absence of removal torque difference between the values of the screws within each group (intragroup analysis—H0 nr.2).

3. Results

The raw data of unscrewing for each connecting screw after cyclic loading were used to extrapolate the individual percentage values of preload loss used for statistical analysis. The results are shown in Table 1:

Table 1. Unscrewing values and percentages of preload loss obtained for each group.

| | GR.CTR Screwed at 25 Ncm | | | | GR.1 Screwed at 25 Ncm | | | GR.2 Screwed at 25 Ncm | | |
|-------------------|-----------------------------|------------------|------------------|------------------|---------------------------|------------------|--------------|---------------------------|------------------|--|
| | 33 | 43 | 36 | 46 | 33 | 36 | 46 | 36 | 46 | |
| First unscrewing | 16 Ncm = 36% | 14 Ncm = 44% | 13 Ncm = 48% | 12 Ncm = 52% | 12 Ncm = 52% | 15 Ncm = 40% | 15 Ncm = 40% | 13 Ncm = 48% | 12 Ncm = 52% | |
| Second unscrewing | 15 Ncm = 40% | 14 Ncm = 44% | 13 Ncm = 48% | 13 Ncm = 48% | 18 Ncm = 28% | 18 Ncm = 28% | 15 Ncm = 40% | 15 Ncm = 40% | 12 Ncm = 52% | |
| Third unscrewing | 14 Ncm = 44% | 14 Ncm = 44% | 15 Ncm = 40% | 13 Ncm = 48% | 13 Ncm = 48% | 16 Ncm = 36% | 15 Ncm = 40% | 18 Ncm = 28% | 16 Ncm = 36% | |
| Fourth unscrewing | 17 Ncm = 32% | 15 Ncm = 40% | 11 Ncm = 56% | 16 Ncm = 36% | 11 Ncm = 56% | 18 Ncm = 28% | 15 Ncm = 40% | 16 Ncm = 36% | 16 Ncm = 36% | |
| Second unscrewing | 16 Ncm = 36% | 10 Ncm = 60% | 15 Ncm = 40% | 16 Ncm = 36% | 12 Ncm = 52% | 18 Ncm = 28% | 15 Ncm = 40% | 10 Ncm = 60% | 12 Ncm = 52% | |
| SD | 1.14 Ncm = 4.56% | 1.95 Ncm = 7.80% | 1.67 Ncm = 6.69% | 1.87 Ncm = 7.48% | 2.77 Ncm = 11.10% | 1.41 Ncm = 5.66% | 0 | 2.52 Ncm = 12.20% | 2.31 Ncm = 8.76% | |
| Mean | 15.6 Ncm = 37.6% | 13.4 Ncm = 46.4% | 13.4 Ncm = 46.4% | 14 Ncm = 44% | 13.2 Ncm = 47.2% | 17 Ncm = 32% | 15 Ncm = 40% | 14.4 Ncm = 42.4% | 13.6 Ncm = 45.6% | |

From one-way ANOVA with Bonferroni correction, the following results were obtained:

- There were no significant statistical differences in torque mean values between Gr.1, Gr.2, and Gr.CTR (*p*-value = 0.2670).
- There were no significant statistical differences between the percentages of preload loss for the screw in position 36 between the three different groups (*p*-value = 0.0569).
- There were no significant statistical differences between the percentages in preload loss for the screw in position 46 between the three different groups (*p*-value = 0.4177).
- The difference between the screws in positions 36 and 46 and 33 and 46 in Gr.1 showed no statistically significant difference, with *p*-value = 0.0193.
- A statistically significant difference between the percentages of preload loss between the screws in positions 33 and 36 in Gr.1 was found equal to 15.2% (*p*-value = 0.0176) (Table 2).
- There was no statistical significant difference between the percentages of torque loss between screws in positions 33 and 46 (*p*-value = 0.4184) and between screws in positions 36 and 46 (*p*-value = 0.3123) in Gr.1.

Table 2. One way ANOVA test for GR.1. In yellow, are the results of the statistic comparisons between the screws in positions 33 and 36.

| Bonferroni's Multiple Comparisons Test | Mean Diff | 95.00% CI of Diff | Below Threshold? | Summary | Adjusted <i>p</i> Value | |
|--|-----------|-------------------|------------------|------------|-------------------------|-----|
| 33 vs. 36 | 15.20 | 2.556 to 27.84 | Yes | * | 0.0176 | A–B |
| 33 vs. 46 | 7.200 | −5.444 to 19.84 | No | ns | 0.4184 | A–C |
| 36 vs. 46 | −8.000 | −20.64 to 4.644 | No | ns | 0.3123 | B–C |
| Test details | Mean 1 | Mean 2 | Mean Diff | SE of diff | n1 | n2 |
| 33 vs. 36 | 47.20 | 32.00 | 15.20 | 4.549 | 5 | 5 |
| 33 vs. 46 | 47.20 | 40.00 | 7.200 | 4.549 | 5 | 5 |
| 36 vs. 46 | 32.00 | 40.00 | −8.000 | 4.549 | 5 | 5 |

Student's *t*-test indicated that:

- There were no statistically significant differences between Gr.1 and Gr.CTR for the screw in position 33 (*p*-value = 0.1114).
- A *p*-value = 0.6465 was calculated, and therefore there was no statistical significant difference between the individual screws 36 and 46 within Gr.2.

4. Discussion

Abutments used for implant-supported prosthodontics have been largely studied, and nowadays the most used solutions are the screw-retained abutments. The use of this type of abutments and their mechanical complications, like the loss of preload and the fracture of prosthetic screws, are well known [31]. The stability of the OT Bridge system is provided by both the screw and the interlocking system between the acetabular Seeger in the extragrade abutment and the subequatorial region of the OT equator attachment. Only few works have been carried on this system out, and research and predictable protocols are only at the beginning, but the clinical results seem to be promising. However, studies on the follow-up period and the number of cases reported with “all-on-four” rehabilitation using the OT bridge system are limited [22–24]. No studies have been proposed to evaluate the influence of removing one or two anterior screws in an “all-on-four” rehabilitation and the stability of this specific system after mechanical loading. This condition can be considered a realistic clinical case where, for esthetic issues, the clinician may choose to avoid the screw hole on one or two anterior implants. In this way, the system is more stressed because the tensile force, resulting from the applied posterior loadings, is counteracted only by the retention capacity of the Seeger. Furthermore, in this study we chose positions 36 and 46 to apply the cyclic loads in order to examine the worst-case condition of loading (on the distal cantilever).

Regarding the results of this study, no statistically differences in mean torque loss values were found between the groups tested, so the null hypothesis (H0 nr.1) was accepted. On the other hand, the null hypothesis for the intra-groups evaluation (H0 nr.2) was not accepted because of the statistically significant difference within Gr.1 between the prosthetic screws in positions 33 and 36.

The absence of statistically significant differences between Gr.1, Gr.2, and Gr.CTR seems to indicate that the OT bridge system could passivate the cyclic loading forces without compromising the entire implant–prosthetic connection even in case of higher mechanical stress than in the normal configuration, such as that occurring in the absence of one tightening screw. Similar results were obtained by Cervino et al. [24] who confirmed the stability of the OT Bridge system in the absence of one screw in an “all-on-four” rehabilitation in a FEM analysis.

From the comparison of the values of Gr.1 (three screws inserted), a statistically significant difference could be noted between the screws in positions 33 and 36 but not between the screws in positions 33 and 46 and 36 and 46 (Table 2).

For the distal 36 and 46 screws, where the loading cycle forces were vertically dissipated (in compression), the OT Bridge system appeared to guarantee stability, because a

significant preload loss was not observed even when one or two anterior prosthetic screws were removed. There were also no differences between the two distal screws in the same model with or without the mesial homolateral screw.

In the model with three screws (Gr.1), the screw in position 33 was more stressed by the loading cycles. Probably, the tensile force, exerted by the lever arm of the distal cantilever in positions 36 and 46, acting in the opposite direction to that of the preloading force of the screw, induced more stress on screw 33. This fact could not be appreciated in the Control Group because of the presence of the second anterior screw (43) that divided the lever arm into additional parts compared to Gr.1. Considering these values, the OT Bridge system seems to be able to dissipate the force even in situations where the mechanical stress should result in a greater overload (model with three screws instead of four).

In this way, it seemed that the Seeger maintained the prosthesis stable and fixed through its retentive action even in the absence of its anterior connection screws (43, 33), as observed for a system with all four screws in place (Gr.CTR).

Theoretically, the removal of one or two connecting screws should lead to an overload on the remaining screws and therefore a loss of preload which, from the analysis conducted, did not occur. This could probably depend on the “Seeger action” which was kept in place, thus being able to carry out its retentive action on the abutment even in the absence of the connection screw.

In support of this thesis, the system was forced beyond the recommended limits by removing the two front screws (33, 43) in Gr.2. This is not a recommended clinical condition, but through the tests we performed, no statistically significant differences for the preload loss between Gr.2 and Gr.CTR were found. In this way, by keeping in place the acetalic Seeger also in the absence of one or two screws, the OT Bridge retentive capacity seems to hinder the loss of preload forces.

The limits of this study are principally related to its *in vitro* nature because the resin model tested did not allow us to understand and determine the effect on soft and hard peri-implant tissues and the number of five unscrewing sessions per group resulted in a limited amount of data. The model used for this study was based on an edentulous lower arch, but for the upper jaws the results could be different because of the different circle arch described and the different implant angulations [22,31]. On the other hand, the bilateral forces exerted on the cantilever to simulate stressful conditions in the oral cavity may be unrealistic, because the chewing function foresees different loading conditions and is multidirectional, not vector-specific. The bilateral cyclic load was performed to test the entire system in a more stressful condition. Another important limit is the lack of data on the Seeger deformation and the holding capacity of the Seeger after cyclic loadings. This could be examined in further research. Additional *in vitro*, *in vivo*, and clinical trials with long-term follow-up, larger samples and different conditions are therefore required to better understand the feasibility of the OT Bridge system.

5. Conclusions

In conclusion, from the results of this *in vitro* study, the OT Bridge seems to be a stable system when using three screws in the “all-on-four” technique applied to a mandibular model. This *in vitro* finding could suggest a good way to solve the esthetic problem of the screw buccal access hole for “screw-retained” fixed solutions, maintaining the advantages of these types of rehabilitations. The mean torque loss values were not statistically different for the groups tested.

The retentive function mediated by the Seeger is useful to maintain the retention of a prosthesis even in mechanical stress conditions. However, different loading conditions, number of cyclic loads, frequency and positions of the applied loads have to be evaluated in the future in order to better understand the OT Bridge system stability.

Author Contributions: Conceptualization, S.C. and F.G.; methodology, S.C.; software, F.T.; validation, M.C.P. and E.M.Z.; formal analysis, M.C.P.; investigation, M.C.P. and F.G.; resources, M.C.P.; data curation, F.G.; writing—original draft preparation, M.C.P.; writing—review and editing, S.C., M.C. and F.G.; visualization, F.T. All authors have read and agreed to the published version of the manuscript.

Funding: This research received no external funding.

Institutional Review Board Statement: Not applicable.

Informed Consent Statement: Not applicable.

Data Availability Statement: Not applicable.

Acknowledgments: The authors thank Rhein83 SRL for supporting this study by furnishing all the necessary materials. The authors would also thank Simone Fedi CDT and New Ancorvis, who projected and fabricated the Cr-Co Milled Framework.

Conflicts of Interest: The authors declare no conflict of interest.

References

- Soto-Peñaloza, D.; Zaragoza-Alonso, R.; Peñarrocha-Diago, M.; Peñarrocha-Diago, M. The all-on-four treatment concept: Systematic review. *J. Clin. Exp. Dent.* **2017**, *9*, e474–e488. [[CrossRef](#)] [[PubMed](#)]
- Moraschini, V.; Poubel, L.D.C.; Ferreira, V.; Barboza, E.D.S. Evaluation of survival and success rates of dental implants reported in longitudinal studies with a follow-up period of at least 10 years: A systematic review. *Int. J. Oral Maxillofac. Surg.* **2015**, *44*, 377–388. [[CrossRef](#)] [[PubMed](#)]
- Maló, P.; Nobre, M.D.A.; Lopes, A.; Francischone, C.; Rigolizzo, M. “All-on-4” Immediate-Function Concept for Completely Edentulous Maxillae: A Clinical Report on the Medium (3 Years) and Long-Term (5 Years) Outcomes. *Clin. Implant Dent. Relat. Res.* **2012**, *14* (Suppl. 1), e139–e150. [[CrossRef](#)] [[PubMed](#)]
- Maló, P.; Rangert, B.; Nobre, M. “All-on-Four” Immediate-Function Concept with Brånemark System® Implants for Completely Edentulous Mandibles: A Retrospective Clinical Study. *Clin. Implant Dent. Relat. Res.* **2003**, *5* (Suppl. 1), 2–9. [[CrossRef](#)] [[PubMed](#)]
- Duyck, J.; Van Oosterwyck, H.; Sloten, J.V.; De Cooman, M.; Puers, R.; Naert, I. Magnitude and distribution of occlusal forces on oral implants supporting fixed prostheses: An in vivo study. *Clin. Oral Implant. Res.* **2000**, *11*, 465–475. [[CrossRef](#)]
- Shadid, R.; Sadaqa, N. A Comparison Between Screw- and Cement-Retained Implant Prostheses. A Literature Review. *J. Oral Implant.* **2012**, *38*, 298–307. [[CrossRef](#)]
- Ortensi, L.; Ortensi, M.; Minghelli, A.; Grande, F. Implant-Supported Prosthetic Therapy of an Edentulous Patient: Clinical and Technical Aspects. *Prosthesis* **2020**, *2*, 140–152. [[CrossRef](#)]
- Pellegrino, G.; Basile, F.; Relics, D.; Ferri, A.; Grande, F.; Tarsitano, A.; Marchetti, C. Computer-Aided Rehabilitation Supported by Zygomatic Implants: A Cohort Study Comparing Atrophic with Oncologic Patients after Five Years of Follow-Up. *J. Clin. Med.* **2020**, *9*, 3254. [[CrossRef](#)]
- Gonçalves, F.; Lucia, V.; Campestrini, L.; Rigo-Rodrigues, M.A.; Rocha Zanardi, P. Effect of the Attachment System on the Biomechanical and Clinical Performance of Overdentures: A Systematic Review. *J. Prosthet. Dent.* **2020**, *123*, 589–594. [[CrossRef](#)]
- Nithyapriya, S.; Ramesh, A.; Kirubakaran, A.; Mani, J.; Raghunathan, J. Systematic analysis of factors that cause loss of preload in dental implants. *J. Indian Prosthodont. Soc.* **2018**, *18*, 189–195. [[CrossRef](#)]
- Byrne, D.; Jacobs, S.; O’Connell, B.; Houston, F.; Claffey, N. Preloads Generated with Repeated Tightening in Three Types of Screws Used in Dental Implant Assemblies. *J. Prosthodont.* **2006**, *15*, 164–171. [[CrossRef](#)] [[PubMed](#)]
- Pjetursson, B.E.; Brägger, U.; Lang, N.P.; Zwahlen, M. Comparison of survival and complication rates of tooth-supported fixed dental prostheses (FDPs) and implant-supported FDPs and single crowns (SCs). *Clin. Oral Implant. Res.* **2007**, *18* (Suppl. 3), 97–113. [[CrossRef](#)] [[PubMed](#)]
- Goodacre, C.J.; Bernal, G.; Rungcharassaeng, K.; Kan, J.Y. Clinical complications with implants and implant prostheses. *J. Prosthet. Dent.* **2003**, *90*, 121–132. [[CrossRef](#)]
- Pellegrino, G.; Grande, F.; Ferri, A.; Pisi, P.; Gandolfi, M.G.; Marchetti, C. Three-Dimensional Radiographic Evaluation of the Malar Bone Engagement Available for Ideal Zygomatic Implant Placement. *Methods Protoc.* **2020**, *3*, 52. [[CrossRef](#)]
- Sailer, I.; Mühlemann, S.; Zwahlen, M.; Hämmerle, C.H.; Schneider, D. Cemented and screw-retained implant reconstructions: A systematic review of the survival and complication rates. *Clin. Oral Implant. Res.* **2012**, *23* (Suppl. 6), 163–201. [[CrossRef](#)] [[PubMed](#)]
- Catapano, S.; Ferrari, M.; Mobilio, N.; Montanari, M.; Corsalini, M.; Grande, F. Comparative Analysis of the Stability of Prosthetic Screws under Cyclic Loading in Implant Prosthodontics: An In Vitro Study. *Appl. Sci.* **2021**, *11*, 622. [[CrossRef](#)]
- Davoudi, A.; Rismanchian, M. Effects of modifying implant screw access channels on the amount of extruded excess cement and retention of cement-retained implant-supported dental prostheses: A systematic review. *J. Prosthet. Dent.* **2018**, *121*, 52–58. [[CrossRef](#)]
- Wittneben, J.G.; Joda, T.; Weber, H.P.; Brägger, U. Screw retained vs. cement retained implant-supported fixed dental prosthesis. *Periodontology 2000* **2017**, *73*, 141–151. [[CrossRef](#)]

19. Mobilio, N.; Catapano, S. Use of monolithic lithium disilicate for implant abutment and crown: A clinical report. *J. Osseointegration* **2019**, *11*, 504–506. [[CrossRef](#)]
20. Mobilio, N.; Fasiol, A.; Catapano, S. Survival Rates of Lithium Disilicate Single Restorations: A Retrospective Study. *Int. J. Prosthodont.* **2018**, *31*, 283–286. [[CrossRef](#)]
21. Mobilio, N.; Catapano, S. The use of monolithic lithium disilicate for posterior screw-retained implant crowns. *J. Prosthet. Dent.* **2017**, *118*, 703–705. [[CrossRef](#)] [[PubMed](#)]
22. Kher, U.; Tunkiwal, A.; Patil, P.G. Management of unfavorable implant positions and angulations in edentulous maxillae with different complete-arch fixed prosthetic designs: A case series and clinical guidelines. *J. Prosthet. Dent.* **2020**, *127*, 6–14. [[CrossRef](#)] [[PubMed](#)]
23. Acampora, R.; Montanari, M.; Scarscia, R.; Ferrari, E.; Pasi, M.; Cervino, G.; Meloni, S.M.; Lumbau, A.I.; Khanari, E.; Koshovari, A.; et al. 1-Year Evaluation of OT Bridge Abutments for Immediately Loaded Maxillary Fixed Restorations: A Multi-center Study. *Eur. J. Dent.* **2021**, *15*, 290–294. [[CrossRef](#)] [[PubMed](#)]
24. Cervino, G.; Ciccì, M.; Fedi, S.; Milone, D.; Fiorillo, L. FEM Analysis Applied to OT Bridge Abutment with Seeger Retention System. *Eur. J. Dent.* **2021**, *15*, 47–53. [[CrossRef](#)] [[PubMed](#)]
25. Rodriguez, A.M.; Aquilino, S.A.; Lund, P.S. TOPICS OF INTEREST Cantilever and implant biomechanics: A review of the literature, Part 2. *J. Prosthodont.* **1994**, *3*, 114–118. [[CrossRef](#)]
26. Storelli, S.; Del Fabbro, M.; Scanferla, M.; Palandrani, G.; Romeo, E. Implant-supported cantilevered fixed dental rehabilitations in fully edentulous patients: Systematic review of the literature. Part II. *Clin. Oral Implant. Res.* **2018**, *29*, 275–294. [[CrossRef](#)]
27. Sistemi Di Prova Elettrodinamici MTS Acumen ® Fornire Modi Più Silenziosi, Semplici e Rapidi per Ottenere Dati Migliori. Available online: <https://www.mts.com/it/products/materials/dynamic-materials-test-systems/acumen-electrodynamic> (accessed on 18 January 2022).
28. Wiskott, H.W.; Nicholls, J.I.; Belser, U.C. Stress fatigue: Basic principles and prosthodontic implications. *Int. J. Prosthodont.* **1995**, *8*, 105–116. Available online: <https://pubmed.ncbi.nlm.nih.gov/7575960/> (accessed on 18 January 2022).
29. Zhu, Y.; Hsu, W.H.; Hollis, J.H. Increasing the number of masticatory cycles is associated with reduced appetite and altered postprandial plasma concentrations of gut hormones, insulin and glucose. *Br. J. Nutr.* **2013**, *110*, 384–390. [[CrossRef](#)]
30. Gaddale, R.; Mishra, S.K.; Chowdhary, R. Complications of screw- and cement-retained implant-supported full-arch restorations: A systematic review and meta-analysis. *Int. J. Oral Implantol.* **2020**, *13*, 11–40. Available online: <http://www.ncbi.nlm.nih.gov/pubmed/32186285> (accessed on 18 January 2022).
31. de Carvalho, L.P.; de Carvalho, A.M.; Francischone, C.E.; Amaral, F.L.B.D.; Sotto-Maior, B.S. Biomechanical behavior of atrophic maxillary restorations using the all-on-four concept and long trans-sinus implants: A finite element analysis. *J. Dent. Res. Dent. Clin. Dent. Prospect.* **2021**, *15*, 106–110. [[CrossRef](#)]