

Broadband Microwave Antenna for Imaging and Sensing in Biomedical Applications

*Original*

Broadband Microwave Antenna for Imaging and Sensing in Biomedical Applications / Portela, D. E.; González, J. F.; Gugliermi, M.; Vipiana, F.; Rodriguez-Duarte, D. O. - ELETTRONICO. - 29:(2024), pp. 2767-2768. ( IEEE International Symposium on Antennas and Propagation and INC/USNCURSI Radio Science Meeting (AP-S/INC-USNC-URSI) Florence (Italy) 14-19 July 2024) [10.1109/ap-s/inc-usnc-ursi52054.2024.10686799].

*Availability:*

This version is available at: 11583/2993296 since: 2024-10-21T19:56:41Z

*Publisher:*

IEEE

*Published*

DOI:10.1109/ap-s/inc-usnc-ursi52054.2024.10686799

*Terms of use:*

This article is made available under terms and conditions as specified in the corresponding bibliographic description in the repository

*Publisher copyright*

IEEE postprint/Author's Accepted Manuscript

©2024 IEEE. Personal use of this material is permitted. Permission from IEEE must be obtained for all other uses, in any current or future media, including reprinting/republishing this material for advertising or promotional purposes, creating new collecting works, for resale or lists, or reuse of any copyrighted component of this work in other works.

(Article begins on next page)

# Broadband Microwave Antenna for Imaging and Sensing in Biomedical Applications

D. E. Portela<sup>(1)</sup>, J. F. González<sup>(1)</sup>, M. Gugliermينو<sup>(2)</sup>, F. Vipiana<sup>(2)</sup>, and D. O. Rodriguez-Duarte<sup>(2)</sup>

<sup>(1)</sup> Universidad Nacional de Colombia, Bogotá, Colombia

<sup>(2)</sup> Dept. Electronics and Telecommunications, Politecnico di Torino, Torino, Italy (david.rodriguez@polito.it)

**Abstract**—Thanks to their operation band, broadband antennas demonstrate applicability and versatility in biomedical sensing and imaging. This work presents the numerical validation of a microwave broadband monopole antenna aimed for work in close proximity to biological tissues, such as the human head. An iterative design starting from an elliptical patch antenna reduces geometry dimensions and enhances bandwidth efficiency. The final design achieves a compact  $48 \times 38$  mm antenna with a dielectrically custom-made 3 mm-thickness matching layer covering a  $-10$  dB frequency band from 1 to 6 GHz, which is assessed on top of a simplified multi-layer head phantom.

## I. INTRODUCTION

The need for cost-effective and accessible systems without ionizing radiation exposure has driven the use of microwave-based solutions for biomedical issues. Applications include microwave imaging for stroke and breast cancer diagnosis, blood glucose monitoring, and pleural effusion detection [1]–[5]. The success of these microwave-based alternatives hinges significantly on the design of the radiating element, a critical factor influencing resolution and penetration, as well as determining factor on the selection of the data processing algorithm.

Various antenna architectures have been proposed for biomedical applications, with wide band antennas standing out as versatile solutions. However, a notable technical challenge lies in their realistic close-body operation conditions impacting directly on antenna performance.

In this study, we present a broadband monopole antenna design, stressing the reduction of antenna dimensions and improving bandwidth efficiency while works near biological tissues. We investigated an elliptical patch antenna, techniques for enhancing bandwidth and the integration of a manufacturable custom-made matching medium (MM).

## II. DESIGN PROCESS

A multi-purpose monopole antenna featuring an operating band from 1 to 6 GHz is proposed, covering the bands used by microwave imaging and sensing applications [2]–[5]. The ground design incorporates a slot antenna with a clipped ground plane printed on a 1.59 mm Rogers RT5880 substrate [6]. Moreover, it considers the antenna’s surrounding effects on the near-field and performance. For this purpose, a layered model —comprising skin, bone, cerebrospinal fluid (CSF), and brain— is employed, assigning their respective dielectric properties [7]. The thickness of each layer was selected according to [8], resulting in a block of homogeneous layers that size is  $96 \times 76 \times 161.7$  mm, as shown in Fig. 1(a).

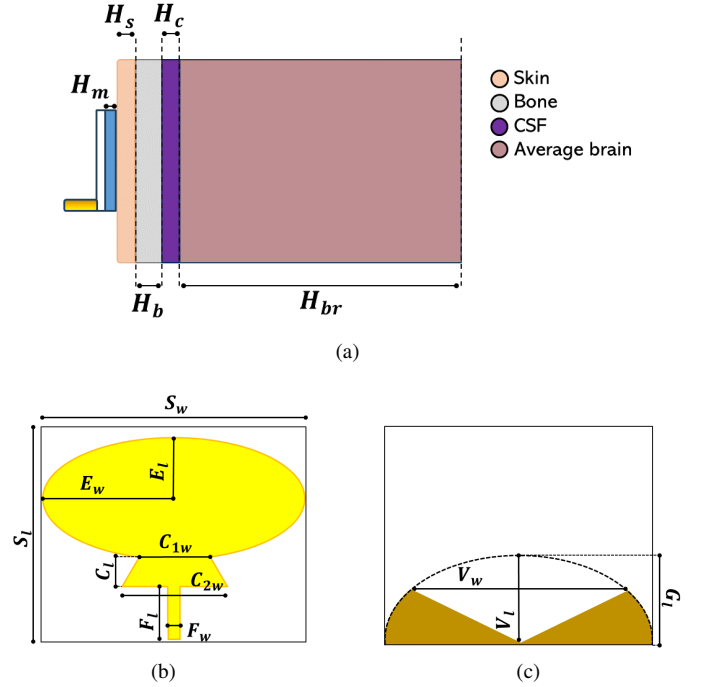


Fig. 1. Numerical models. (a) Head model and antenna setup, including the matching medium in blue. (b-c) Proposed antenna, front and back view, respectively.

Following the establishment of the initial patch antenna model, iterative simulations achieve the goal of a wide bandwidth starting from 1 GHz. The first iteration involves modifying the radiator element into an elliptical shape and introducing slots in the ground plane, following the approach proposed in [9]. This enhanced matching at lower frequencies. Subsequently, a slot is added to the ground plane, improving higher frequencies as suggested in [10], resulting in an enhanced coupling across the full band.

As the antenna dimensions are reduced, operating frequencies tend to increase, requiring new strategies for adapting coupling at the desired points. Then, the addition of stubs to the feed line is explored, initially with a single stub, leading to an overall low-frequency performance increment. The introduction of a second symmetrical stub revealed a second resonance point at 1 GHz, emphasizing the importance of a smooth transition from the feed line to the radiator. The final structure was triangular, seamlessly transitioning between the strip line and the ellipse.

Additional simulations were conducted to determine the optimal size of the ground plane, revealing that a slightly larger ground plane with a deeper slot enhances coupling across the entire bandwidth. The resulting design, achieved through this iterative process, has dimensions of  $61 \times 43$  mm, representing a significant reduction compared to the initial design, but falling behind the goal of a minimum size of  $50 \times 40$  mm.

Finally, a triangular structure was integrated into the feed line and radiator to achieve a compact antenna design. Moreover, as the last iteration, a MM is introduced between the antenna and the head phantom, which reduces the dimensions and improves the physical coupling between the antenna and the application zone. For the MM, the degrees of freedom are the thickness and permittivity,  $\epsilon$ , being 3 mm the reached optimal, and  $\epsilon = 17.876 + j2.345$  at 2 GHz, respectively. Here, it is worth notice that the used values correspond to real custom-made dispersive materials, which are made with a mixture of urethane rubber and graphite [11]. The final antenna design yields a  $48 \times 38$  mm antenna, including its radiating element and ground plane as depicted in Fig.1b and 1c, and reported in Table I.

TABLE I  
DIMENSIONS OF PROPOSED ANTENNA AND MULTI-LAYERS PHANTOM

Index	[mm]	Index	[mm]	Index	[mm]
$S_w$	48	$G_l$	20	$S_l$	38
$V_w$	42.72	$S_h$	1.6	$V_l$	19
$C_l$	4	$F_l$	11	$C_{1w}$	14.76
$H_m$	3	$C_{2w}$	20	$H_s$	3
$F_w$	4	$H_b$	6.5	$E_w$	23
$H_c$	3.2	$E_l$	10.5	$H_{br}$	150

### III. RESULTS

The iterative process successfully met the bandwidth requirements, with a wide bandwidth covering from 1 to 6 GHz, positioning it as an attractive choice for applications in body microwave imaging and sensing. The  $S_{1,1}$  parameter results at each step of this procedure are illustrated in Fig. 2, demonstrating progressive enhancement design requirements throughout the iteration process. Notably, although the first iterations performed well, the final design achieved size advantages, particularly crucial for the body microwave imaging application with multiple antennas as in [5].

### IV. CONCLUSIONS AND FUTURE WORK

An ultra-wideband elliptical monopole antenna with partial ground plane clipping is specifically designed for microwave imaging and sensing applications, operating effectively in the frequency range from 1 to 6 GHz. Incorporating a realistic matching medium has been validated, reducing the antenna's size and facilitating better structural adaptation around the area of interest. Considering the promising results of the proposed antenna, in future work is planned to validate it experimentally.

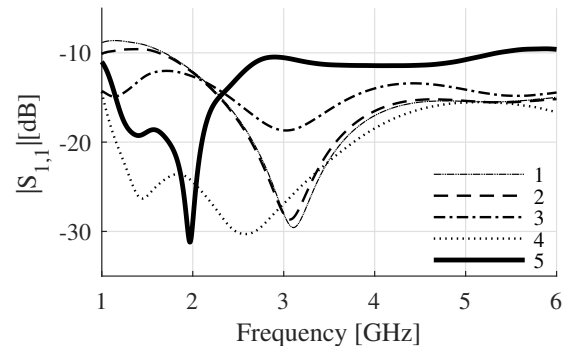


Fig. 2. Reflection coefficient amplitude of the proposed antennas for the different design iterations. The numbers indicate different design iterations.

### ACKNOWLEDGEMENT

This work was supported in part by the Agritech National Research Center, funded by the European Union Next-Generation EU (Piano Nazionale di Ripresa e Resilienza (PNRR) – MISSIONE 4 COMPONENTE 2, INVESTIMENTO 1.4 – D.D. 1032 17/06/2022, CN00000022).

### REFERENCES

- [1] P. Bhardwaj and R. K. Badhai, "Compact wideband folded strip monopole antenna for brain stroke detection," *International Journal of Microwave and Wireless Technologies*, vol. 13, no. 9, pp. 937–946, 2021.
- [2] S. Ullah, C. Ruan, M. S. Sadiq, T. U. Haq, and W. He, "High efficient and ultra wide band monopole antenna for microwave imaging and communication applications," *Sensors*, vol. 20, no. 1, 2020.
- [3] M. Manoufali, A. T. Mobashsher, B. Mohammed, K. Bialkowski, P. C. Mills, and A. Abbosh, "Implantable sensor for detecting changes in the loss tangent of cerebrospinal fluid," *IEEE transactions on biomedical circuits and systems*, vol. 14, no. 3, pp. 452–462, 2020.
- [4] R. Chandra, H. Zhou, I. Balasingham, and R. M. Narayanan, "On the opportunities and challenges in microwave medical sensing and imaging," *IEEE transactions on biomedical engineering*, vol. 62, no. 7, pp. 1667–1682, 2015.
- [5] D. O. Rodriguez-Duarte, C. Origlia, J. A. T. Vasquez, R. Scapaticci, L. Crocco, and F. Vipiana, "Experimental assessment of real-time brain stroke monitoring via a microwave imaging scanner," *IEEE Open Journal of Antennas and Propagation*, vol. 3, pp. 824–835, 2022.
- [6] "Roger 5880," Available at <https://rogerscorp.com/advanced-electronics-solutions/rt-duroid-laminates/rt-duroid-5880-laminates>.
- [7] D. Andreuccetti, R. Fossi, and C. Petrucci, "An internet resource for the calculation of the dielectric properties of body tissues in the frequency range 10 hz - 100 ghz," Available online: <http://niremf.ifac.cnr.it/tissprop/>, 1997.
- [8] K. Wendel, D. Stolar, J. Malmivuo, and J. Hyttinen, "Measuring tissue thicknesses of the human head using centralized and normalized trajectories," in *Proceedings of the conference Consciousness and its Measures*, vol. 29, no. 1.12, 2009.
- [9] M. S. Talukder, M. M. Alam, M. T. Islam, M. Moniruzzaman, R. Azim, A. G. Alharbi, A. I. Khan, M. Moinuddin, and M. Samsuzzaman, "Rectangular slot with inner circular ring patch and partial ground plane based broadband monopole low sar patch antenna for head imaging applications," *Chinese Journal of Physics*, vol. 77, pp. 250–268, 2022.
- [10] P. Okas, A. Sharma, G. Das, and R. K. Gangwar, "Elliptical slot loaded partially segmented circular monopole antenna for super wideband application," *AEU-International Journal of Electronics and Communications*, vol. 88, pp. 63–69, 2018.
- [11] C. Origlia, M. Gugliemino, D. O. Rodriguez-Duarte, J. T. Vasquez, and F. Vipiana, "Anthropomorphic multi-tissue head phantom for microwave imaging devices testing," in *2023 17th European Conference on Antennas and Propagation (EuCAP)*. IEEE, 2023, pp. 1–4.