

International comparison on SST and Epstein measurements in grain-oriented Fe-Si sheet steel

*Original*

International comparison on SST and Epstein measurements in grain-oriented Fe-Si sheet steel / C., A., E., F., F., F., L., R., Ragusa, C.S., J., S., T., B., C., W., P., D., S., S., Y., N., K., G., S., N., R., L., M., A., X., Z., W., F., X., G., M., H.. - STAMPA. - (2014), pp. 21-22. (13th International Workshop on International Workshop on 1&2 DIMENSIONAL MAGNETIC MEASUREMENT AND TESTING 10 - 12 September 2014 Torino, Italy Torino 10 - 12 September 2014).

*Availability:*

This version is available at: 11583/2588569 since: 2021-03-27T12:37:59Z

*Publisher:*

Politecnico di Torino

*Published*

DOI:

*Terms of use:*

This article is made available under terms and conditions as specified in the corresponding bibliographic description in the repository

*Publisher copyright*

(Article begins on next page)

## International comparison on SST and Epstein measurements in grain-oriented Fe-Si sheet steel

C. APPINO<sup>1</sup>, E. FERRARA<sup>1</sup>, F. FIORILLO<sup>1</sup>, L. ROCCHINO<sup>1</sup>, C. RAGUSA<sup>2</sup>, J. SIEVERT<sup>3</sup>, T. BELGRAND<sup>4</sup>, C. WANG<sup>5</sup>, P. DENKE<sup>6</sup>, S. SIEBERT<sup>6</sup>, Y. NORGREN<sup>7</sup>, K. GRAMM<sup>7</sup>, S. NORMAN<sup>8</sup>, R. LYKE<sup>8</sup>, M. ALBRECHT<sup>9</sup>, X. ZHOU<sup>10</sup>, W. FAN<sup>11</sup>, X. GUO<sup>12</sup>, M. HALL<sup>13</sup>

<sup>1</sup>INRIM, Torino, Italy, <sup>2</sup>Politecnico di Torino, Italy, <sup>3</sup>PTB (former affiliation), Braunschweig, Germany, <sup>4</sup>TKES, Isbergues, France, <sup>5</sup>TKES, Gelsenkirchen, Germany, <sup>6</sup>BROCKHAUS Messtechnik, Lüdenscheid, Germany, <sup>7</sup>ABB, Ludvika, Sweden, <sup>8</sup>AK Steel, Middletown, USA, <sup>9</sup>PTB, Braunschweig, Germany, <sup>10</sup>BAOSTEEL, Shanghai, China, <sup>11</sup>NIM, Beijing, China, <sup>12</sup>WISCO, Wuhan, China, <sup>13</sup>NPL, Teddington, UK.  
(c.appino@inrim.it)

### 1. Introduction

Electrical sheet steels are sold and applied against properties typically measured through either the Epstein or Single Sheet (SST) testing methods, according to the IEC 60404-2 and IEC 60404-3 standards, respectively. Because of the different sample geometries and involved magnetic circuits, these two methods, while both ensuring good reproducibility, do provide different results. The obtained figures of power loss and apparent power, in particular, are in a complex relationship, depending on the type of material, the polarization value, the test frequency, the lamination thickness, and, for the SST method, the quality of the flux-closing yoke [1]. The problem bears special importance for grain-oriented (GO) Fe-Si grades, where the differences are larger. A previous investigation, performed by one metrological laboratory on a very large number of samples, led to an empirical power law for the relative difference of the 50 Hz power losses  $\delta P_{SE} = (P_{SST} - P_{Eps}) / P_{Eps}$  versus the polarization value [2]. This was accounted for through an informative annex to the IEC 60404-3 standard. However, it was also recognized that significant statistical evaluation of the Epstein-SST relationship and its possible physical assessment could be achieved only through an international comparison exercise involving a suitably high number of metrological and industrial laboratories. A new IEC project was then started, where samples belonging to five different grades of GO laminations were circulated among ten different laboratories. In this communication we shall provide the main results and the statistical analysis of this comparison.

### 2. Methods and Results

Five different GO grades, with nominal thickness ranging between 0.23 mm and 0.30 mm, were tested by the participating laboratories according to the IEC 60404-2 and IEC 60404-3 standards. The power loss and the apparent power were measured at 20, 40, 50, 60, 80, 100 Hz for peak polarization values  $J = 1.3, 1.5, 1.7, \text{ and } 1.8 \text{ T}$ . Each laboratory was assumed to have appropriate traceability of measurements and was required to determine the measurement uncertainty according to the ISO/IEC Guide [3]. Fig. 1 shows the experimental relative standard deviation  $s_p$  of the laboratories reported values around the mean  $\langle P_{Eps} \rangle$  and  $\langle P_{SST} \rangle$  of the 50 Hz power

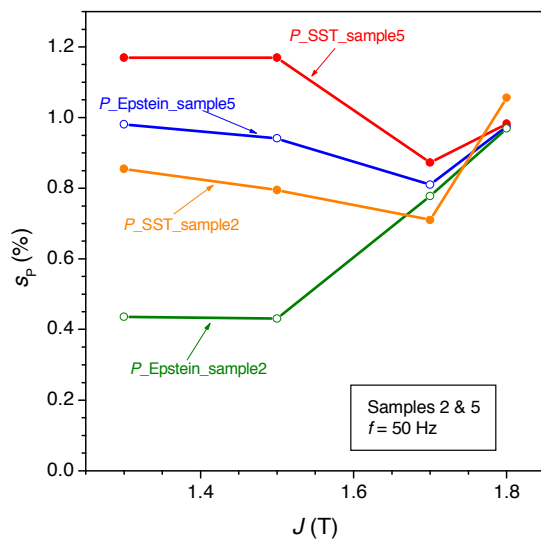


Fig. 1 - Experimental standard deviation  $s_p$  of the laboratory best estimates of the Epstein and SST 50 Hz power loss measurements (samples 2 and 5).

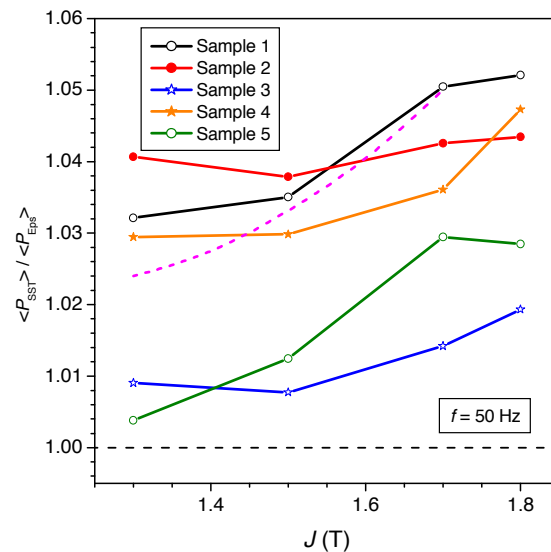


Fig. 2 - Ratio  $\langle P_{SST} \rangle / \langle P_{Eps} \rangle$  of the mean values of the measured SST and Epstein 50 Hz power losses. The dashed line is the least square fit of previous literature results, used in the informative annex to IEC 60404-3) [2].

loss for two representative samples. These show the highest (sample 2) and the lowest (sample 5), loss figures, respectively.  $s_p$  is at most 1.2 % and it ranges, in particular, between 0.7 % and 0.9 % at  $J = 1.7$  T. On the other hand, Fig. 2 shows that the ratio  $\langle P_{SST} \rangle / \langle P_{Eps} \rangle$  is greater than 1 everywhere and increases with  $J$ . The conventional GO materials (samples 1, 2, 4) are observed to follow fairly well the average  $\langle P_{SST} \rangle / \langle P_{Eps} \rangle$  trend (dashed line in Fig. 2) obtained in previous experiments and proposed in the informative annex to IEC 60404-3. A lower  $\langle P_{SST} \rangle / \langle P_{Eps} \rangle$  ratio is instead exhibited at all  $J$  values by the high-grade samples 3 and 5. The experiments additionally show that  $\langle P_{SST} \rangle / \langle P_{Eps} \rangle$  tends to decrease with the increase of the magnetizing frequency. Similar trends are observed in the behaviour of the apparent power and the related ratio  $\langle S_{SST} \rangle / \langle S_{Eps} \rangle$ , although on a significantly different scale. For one thing, the experimental standard deviation  $s_s$  is larger than  $s_p$ , especially for the SST measurements. The mean value  $\langle S_{SST} \rangle$  tends then to attain values from a few percent up to about 40% higher than  $\langle S_{Eps} \rangle$  on going from  $J = 1.3$  T to  $J = 1.8$  T. The reason for these large discrepancies is thought to reside in the inevitably different harmonic composition of the supply current signals ensuring sinusoidal secondary voltage in the two different magnetic circuits.

## References

- [1] J. Sievert, The measurement of magnetic properties of electrical sheet steel. Survey of methods and standards, *J. Magn. Magn. Mater.*, **215-216** (2000), 647-651.
- [2] J. Sievert and H. Ahlers, Epstein to SST relationship-statistical rather than deterministic, *Electrical Review*, **9b** (2011), 17-19.
- [3] BIPM, IEC, IFCC, ILAC, ISO, IUPAC, IUPAP, OIML, *Guide to the expression of uncertainty in measurement*, JCGM/WG 1, 2008.