



POLITECNICO DI TORINO  
Repository ISTITUZIONALE

SERS-active metal-dielectric nanostructures integrated in microfluidic devices for ultra-sensitive label-free miRNA detection

*Original*

SERS-active metal-dielectric nanostructures integrated in microfluidic devices for ultra-sensitive label-free miRNA detection / CHIADO', ALESSANDRO; NOVARA, CHIARA; LAMBERTI, ANDREA; GEOBALDO, FRANCESCO; GIORGIS, FABRIZIO; RIVOLO, PAOLA. - In: *PROCEDIA TECHNOLOGY*. - ISSN 2212-0173. - *ELETTRONICO*. - 27(2017), pp. 37-38.

*Availability:*

This version is available at: 11583/2684061 since: 2017-10-17T19:07:55Z

*Publisher:*

Elsevier

*Published*

DOI:10.1016/j.protcy.2017.04.018

*Terms of use:*

openAccess

This article is made available under terms and conditions as specified in the corresponding bibliographic description in the repository

*Publisher copyright*

(Article begins on next page)

Biosensors 2016

## SERS-active metal-dielectric nanostructures integrated in microfluidic devices for ultra-sensitive label-free miRNA detection

Chiadò A.<sup>a\*</sup>, Novara C.<sup>a</sup>, Lamberti A.<sup>a</sup>, Geobaldo F.<sup>a</sup>, Giorgis F.<sup>a</sup>, Rivolo P.<sup>a</sup>

*<sup>a</sup>Department of Applied Science and Technology, Politecnico di Torino, Corso Duca degli Abruzzi 24, 10129 Torino, Italy*

---

### Abstract

In this work, silver decorated porous silicon membranes integrated in a polydimethylsiloxane multi-chamber microfluidic chip were functionalized with DNA-probes and used for the detection of miRNA by Surface-enhanced Raman Scattering analysis. An innovative biological protocol has been designed: the probe was divided in two short pieces that interact before and after the miRNA incubation. The optofluidic biosensor was applied for the label-free detection of miRNA sequences at *in vivo* concentrations.

© 2017 The Authors. Published by Elsevier Ltd. This is an open access article under the CC BY-NC-ND license (<http://creativecommons.org/licenses/by-nc-nd/4.0/>).

Peer-review under responsibility of the organizing committee of Biosensors 2016

*Keywords:* "Surface Enhanced Raman Scattering; miRNA; ELISA; optofluidic biosensor; metal-dielectric nanostructures; porous silicon;"

---

### 1. Introduction

Surface-enhanced Raman Scattering (SERS) plays an important role in the high-sensitive label-free detection of biomolecules. Nanostructured materials based on semiconductors and metal-oxides decorated by noble metal nanoparticles have been recently developed as SERS-active substrates [1,2].

In this work SERS is applied for the detection of miRNA, which consist of short regulatory sequences usually over- or under- expressed in connection with a particular disease (e.g. oncogenesis) [3]. In detail, new ultra-sensitive metal-dielectric substrates made of silver decorated porous silicon (pSi) membranes were functionalized and used to detect different miRNA sequences in a polydimethylsiloxane (PDMS) multichamber microfluidic chip.

---

\* Corresponding author. Tel.: +390110907370; fax: +390110907399.

*E-mail address:* [alessandro.chiado@polito.it](mailto:alessandro.chiado@polito.it)

## 2. Experimental

The synthesis of the PDMS-supported Ag-pSi membranes (PSD) and of the PDMS multichamber microfluidic chip is reported elsewhere [2]. A protocol for miRNA detection performed by enzyme-linked immunosorbent assay (ELISA) was set-up on commercial plates by the overnight immobilization of a 5'-alkylthiol-capped DNA probe (25  $\mu$ M, in TE, 1 M NaCl, pH 7.5) corresponding to the antisense sequence of the miRNA222. The hybridization (22  $^{\circ}$ C, 60 min) was performed in SSC4x, 0.1% SDS, pH 7.5. Streptavidin-HRP was incubated (22  $^{\circ}$ C, 60 min) to detect biotin and a TMB substrate solution was used for the colorimetric reaction. Subsequently, the biological assay was transferred to the substrates used for SERS analysis with excitation at 514.5 nm.

## 3. Results and Discussion

The protocol developed in commercial ELISA plates was adapted to the PSD substrates and to the optofluidic biosensor (Fig.1a) in two operative approaches. In the first, the hybridization was assessed by incubation of the corresponding miRNA sequence. (Fig.1b). Due to the poor sensitivity of this method, the probe was divided in two pieces (half1 and half2) that interact before and after the miRNA incubation, to allow the label-free miRNA profiling in two hybridization steps (Fig.1c). The half2 was modified with biotin or with a Raman label (cy3). Afterwards, the ELISA and the SERS analysis (Fig.1d-e) were used to assess the hybridization between the grafted probe and the miRNA, allowing its label-free detection in a physiological range of concentrations (0.1-50 nM).

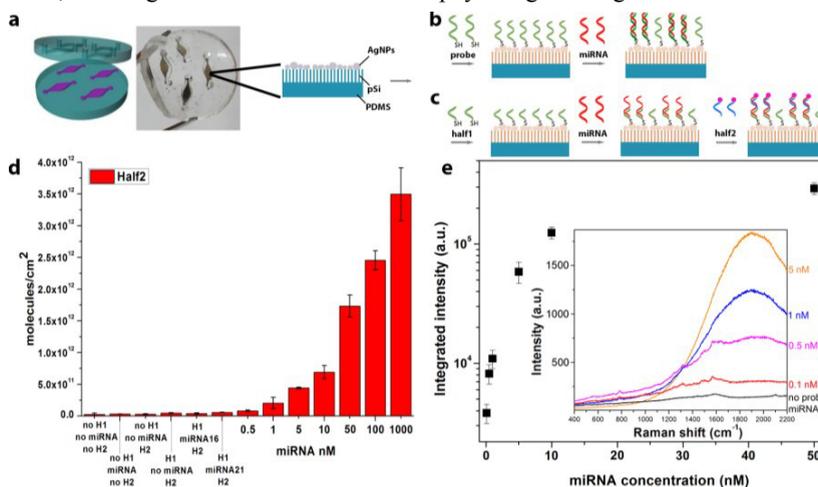


Fig. 1. (a) PDMS multichamber microfluidic chip; (b) one-step hybridization bioassay; (c) two-steps hybridization bioassay; (d) ELISA test performed by two-steps hybridization process; (e) SERS analysis conducted by two-steps hybridization protocol.

## 4. Conclusion

The optimized protocols applied to metal-dielectric nanostructures yielded the label-free detection of miRNA at *in vivo* concentrations, proving the potentialities of SERS-microfluidic chips in the frame of early-cancer diagnosis.

## References

- Lamberti A, Virga A, Chiadò A, Chiodoni A, Bejtka K, Rivolo P, et al. Ultrasensitive Ag-coated TiO<sub>2</sub> nanotube arrays for flexible SERS-based optofluidic devices. *J Mater Chem C*. 2015;3(26):6868–75.
- Novara C, Lamberti A, Chiadò A, Virga A, Rivolo P, Geobaldo F, et al. Surface-enhanced Raman spectroscopy on porous silicon membranes decorated with Ag nanoparticles integrated in elastomeric microfluidic chips. *RSC Adv*. 2016;6(26):21865–70.
- Dong H, Lei J, Ding L, Wen Y, Ju H, Zhang X. MicroRNA : Function, Detection, and Bioanalysis. *Chem Rev*. 2013;113:6207–33.