

Mutual Coupling Reduction between Implanted Microstrip Antennas on a Cylindrical Bio-Metallic Ground Plane

*Original*

Mutual Coupling Reduction between Implanted Microstrip Antennas on a Cylindrical Bio-Metallic Ground Plane / Matekovits, Ladislau; Huang, Jie; Peter, Ildiko; Esselle, Karu P.. - In: IEEE ACCESS. - ISSN 2169-3536. - ELETTRONICO. - 5:(2017), pp. 8804-8811. [10.1109/ACCESS.2017.2703872]

*Availability:*

This version is available at: 11583/2686646 since: 2018-02-27T12:57:22Z

*Publisher:*

Institute of Electrical and Electronics Engineers Inc.

*Published*

DOI:10.1109/ACCESS.2017.2703872

*Terms of use:*

This article is made available under terms and conditions as specified in the corresponding bibliographic description in the repository

*Publisher copyright*

(Article begins on next page)

Received April 8, 2017, accepted May 4, 2017, date of publication May 12, 2017, date of current version June 28, 2017.

Digital Object Identifier 10.1109/ACCESS.2017.2703872

# Mutual Coupling Reduction Between Implanted Microstrip Antennas on a Cylindrical Bio-Metallic Ground Plane

LADISLAU MATEKOVITS<sup>1,2</sup>, (Senior Member, IEEE), JIE HUANG<sup>1</sup>, ILDIKO PETER<sup>3</sup>, AND KARU P. ESSELLE<sup>2</sup>, (Fellow, IEEE)

<sup>1</sup>Department of Electronics and Telecommunications, Politecnico di Torino, 10129 Turin, Italy

<sup>2</sup>School of Engineering, Macquarie University, Sydney, NSW 2109, Australia

<sup>3</sup>Department of Applied Science and Technology, Institute of Science and Engineering of Materials for Innovative Technologies, Politecnico di Torino, 10129 Turin, Italy

Corresponding author: Ildiko Peter (ildiko.peter@polito.it)

**ABSTRACT** The mutual coupling between two antennas within a human body model is studied. Our multilayer cylindrical body model includes highly lossy body tissues under which a biocompatible metal implant is inserted. This cylindrical bio-metal implant serves as the common ground plane for the conformal antennas. The mutual coupling between two such conformal microstrip antennas is studied and quantified for different spacing between them. Three methods are proposed to reduce mutual coupling between the two antennas. Each of them are investigated in details and their effectiveness is compared.

**INDEX TERMS** In-body communication, implanted antenna, mutual coupling.

## I. INTRODUCTION

Medical telemetry, also known as biotelemetry, involves the application of telemetry in medicine and healthcare. It allows remote monitoring of various vital signals in ambulatory patients and it is exploited more and more in the modern healthcare systems. If adequately implemented, i.e., allowing real-time transmission of biological signals from a patient (e.g. temperature, blood pressure, cardiac beat) in a plausible way to a far located medical center, it is possible to distantly monitor a patient and for example to send a medical team only if necessary. The use of such technologies can strongly reduce hospitalization time, and consequently associated costs, without compromising the quality of the service. On the other hand, having the possibility to continuously collect the biological data, it is possible to develop algorithms to predict the evolution of the medical condition of patients, which again can reflect in higher quality of service, for example by considering recovery only when it is necessary.

In some cases, on-body sensors can collect the signals of interest, but in other cases, information has to be obtained from inside the body. In this case, the collected information should be transmitted outward from inside the body. Implanted antennas are the basic elements of any of such system, where communication between an implanted device in the human body with the outside receivers is required.

The location of the implanted antennas depends on the given telemetry application. An example medical telemetry system, with an implanted antenna just under the skin, is detailed in [1]. In other applications, e.g., for a wireless RF powered brain machine interface application, antennas are situated in brain [2], [3]. A planar spiral antenna (PSA) to be placed in the brain to detect the existence of tumor was designed in [3]. The resonant frequency of the PSA is higher in the presence of tumor than for healthy tissues, and this difference can be exploited in the analysis. Other examples are antennas implanted in human arms. In [1] it is shown that the position of the implanted antenna and electrical properties of the insulating layer also affect the RF power reception and the properties of the tissues surrounding the implanted antenna can influence the electrical characteristics of the antennas. Implanted cavity slot antenna with H-shape slot is proposed and characterized in [4].

Few examples of antennas on the bone are in present in the literature. In [5], the reason of using implanted antennas in bone is discussed and a comparison between bone-implanted antenna and a muscle-implanted antenna is presented.

Radiation performances of antennas can be increased, for example, by considering an array of radiators. As for example in [6] where an implanted conformal slot array located between the two parts of a broken femur is considered.

The array solution also presents some drawbacks, such as the larger space required, and the effect of the mutual coupling between the radiators, that can, in turn, reduce the gain or increase the level of sidelobes. In the literature, different ways to reduce the effect of the mutual coupling have been proposed. Methods to reduce mutual coupling between a pair of close E-shaped patch antennas are described in [7], including cutting a slit in the common ground plane. In [8], a parasitic tape on microstrip patch elements was experimented. This mechanism of mutual coupling reduction has been studied by observing the field distribution in the presence of the tape, and comparing with the initial case when the tape is not present. In [9], a solution consisting of the use of a pair of slits between two walls of a printed circuit board in air was studied aiming to improve the isolation of a pair of closely packed antenna elements. In [10], a suspended line that links two planar inverted-F antennas (PIFAs) was used to compensate for coupling. By this way, opposite coupling can be introduced that if properly designed will offset the unwanted interaction and in turn can increase the antenna efficiency. Analogous solution was proposed in [11], where a connection between two ports was considered. Such a solution is convenient and easy to be implemented by appropriately designing the connection. However, the reduction of coupling i.e.,  $S_{21}$  magnitude is accompanied by a shift of the resonant frequency.

Another class of solutions for reducing the mutual coupling between radiators consist of using Electromagnetic Band-gap (EBG) structures. In [12], a periodic structure on a conformal ground plane, which exhibits EBG in the interested band, was used. In [13], a defected ground structure (DGS) with two H-shaped slots between the antennas were used which are placed very closely to each other (distance less than  $0.3\lambda$ ). With this structure, the mutual coupling reduces up to 50 dB without significant influence on the radiation pattern. In [14], a comparison between an EBG structure and DGS structure was performed. However, the study of the mutual coupling for implanted antennas is at the early stage, and to the best of the authors' knowledge, only few examples are reported in the literature.

In this paper, the reduction of the mutual coupling in the case of an implanted two-element antenna array is investigated. The radiators are placed on a metallic cylinder (the implant) embedded in a polymer dielectric that acts as the substrate between the ground plane and radiators, all of them being conformal. Quantification of mutual coupling is performed. For the reduction of mutual coupling, three methods are investigated, and the amount of reduction of coupling with different methods is studied for different positions of the two radiators.

## II. THE BODY MODEL


For the proposed investigation a cylindrical body model is considered. It has dimensions alike to an adult leg. The different tissues modeled as concentric cylinders are characterized by different thicknesses and material parameters (dielectric constant and loss). In all cases the magnetic properties of

tissues and dielectrics have been neglected, i.e. relative magnetic permeability is set to unity. Microwave Studio from CST has been used to model the system and to perform the numerical study.

The material parameters, i.e., relative dielectric constant and conductivity (S/m), are reported in Tab. I.

**TABLE 1. Electrical properties of the body tissues and other material at  $f = 2.45$  GHz.**

	Muscle	Fat	Skin	PDMS layer	Bone /Titanium
Relative permittivity	57.1	5.6	46.7	2.667	Lossy metal
Conductivity (S/m)	0.79	0.04	0.69	0.034	$1e7$

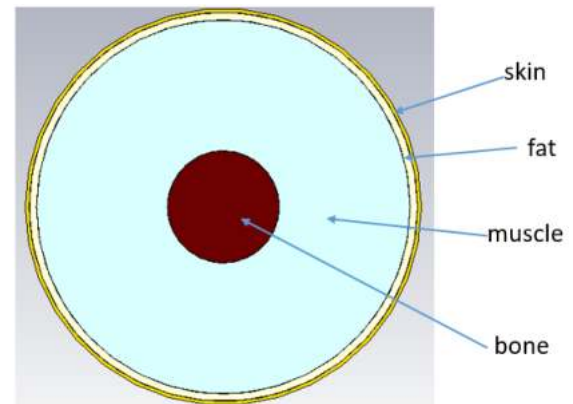


**FIGURE 1. Cross section of the considered model. The “bone” consists of a lossy bio-metal.**

In the considered model in Fig. 1, the central part of the geometry i.e., the bone, is replaced with an implant of the same dimensions made of a biocompatible metal and metallic alloy. Titanium, titanium alloys, stainless steel, cobalt and their alloys can be used for the manufacturing of implant. Generally, in orthopedic field Titanium and its alloys have been employed, because of their excellent biocompatibility, promising mechanical properties and their high corrosion resistance. Ti-6Al-4V is widely used in a variety of stress-bearing orthopedic applications, but some research [15], [16] have demonstrated that occasionally release of Al and V ions arises, with a negative consequence on tissues. In order to avoid such problems, actually the tendency is to employ metallic alloys with no harmful elements, like a basic Ti alloy composition and substituting the hazardous elements by Nb, Ta, Mo, Zr or a combination of them. Porous Ta has been used for hip and knee arthroplasty, while low occurrence of artifacts can be obtained by addition of Ta in TiNi shape memory alloy [17]–[24]. Spongy structures based on glassy alloys with biocompatible elements is proposed in [25] as an alternative solution to the conventional crystalline and amorphous alloys with superior stiffness than human bone. Additionally, the mechanical behaviors as response to mechanical stimulus

like strain and stress, and cell concentrations involving the implant, has also been studied [26].

In this paper, the above mentioned bio-metallic implant is also used as the ground plane for conformal rectangular microstrip antennas, as illustrated in the model in Fig. 2.

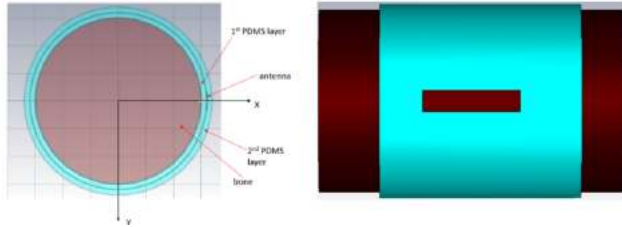

**FIGURE 2.** Location of a conformal rectangular microstrip antenna in between two PDMS layers over the bio-metal implant that has replaced the bone: top view (left), side view with the external PDMS layer removed for a better rendering (right). In both figures the surrounding tissues (muscle, fat and skin) have been removed for a better rendering. They are present in all simulations.

The bio-metal conformal rectangular microstrip antenna is separated from the metallic cylinder ground plane by a conformal substrate made up of Polydimethylsiloxane (PDMS). In the considered model, a second layer of PDMS is also present that acts as superstrate. In the numerical modelling, the thicknesses of the two PDMS layers are considered equal. The dimensions are reported in Tab. II.

**TABLE 2.** The parameters of the model.


Parameter	DESCRIPTION	Value (mm)
$r_{bone}$	radius of the bone	30
$l_{str}$	total length of the implant	100
$l_{PDMS}$	length of each PDMS layer	66
$th_{PDMS}$	thickness of each PDMS layer	2
$th_{muscle}$	thickness of the muscle layer	70
$th_{met}$	thickness of the metal (antenna)	0.5
$th_{fat}$	thickness of the fat layer	4
$th_{skin}$	thickness of the skin layer	2

### III. DESIGN OF THE SINGLE ANTENNA

In the first step of the analysis, a single antenna element has been designed. It is a rectangular microstrip antenna of length  $l_{ant}$  and width  $w_{ant}$ , fed by a probe on its symmetry axis, and at a distance  $l_z$  from one of the edges. The probe is modeled by a metallic cylinder. Its second end is connected to the ground plane (Ti cylinder).

The three aforementioned parameters have been used in an optimization process to minimize the reflection coefficient with respect to a standard  $50 \Omega$  feed at the center of the 2.4 - 2.5 GHz Industrial, Scientific and Medical (ISM) radio band, i.e. at 2.45 GHz. The optimization process was necessary because no analytic formulas for the design that include the body environment are available. After the optimization by a Genetic Algorithm (available in the numerical tool),

the dimensions of the antenna are found to be  $l_{ant} = 32$  mm,  $w_{ant} = 7$  mm and  $l_z = 0$  mm. The corresponding reflection coefficient is shown in Fig. 3.

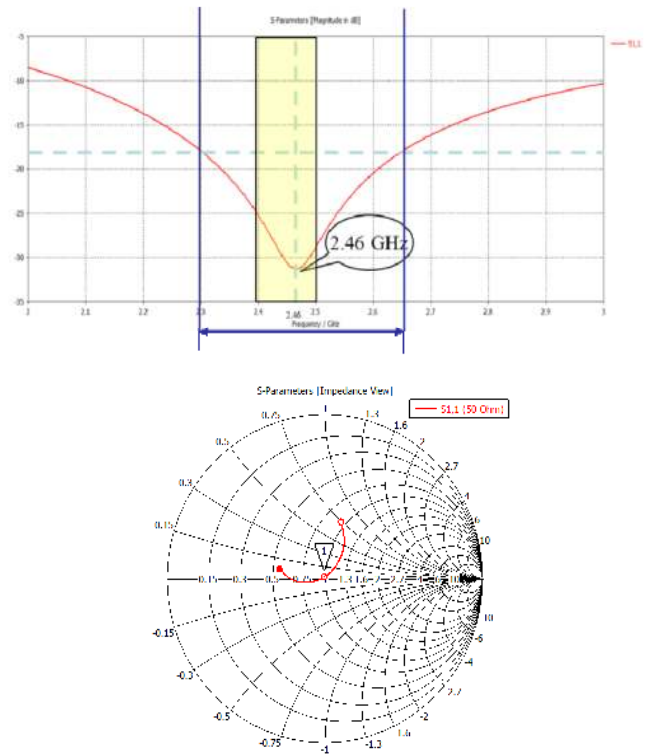


**FIGURE 3.** Reflection coefficient of the optimized antenna. Reference impedance equal to  $50 \Omega$ .

The resulting geometry exhibits good matching at 2.464 GHz, which is close the center of the considered band. The bandwidth is relatively large also due to the losses considered in the modelling.


### IV. MUTUAL COUPLING

As mentioned above, our interest is the quantification of mutual coupling between two antennas. The corresponding scenario is presented in Fig. 4. Two identical antennas are considered. The first one is in a fixed position and the second one is rotated around the implant by an angle  $\alpha$  ( $\alpha$ ), in such a way that it always remains parallel to the cylindrical ground plane.

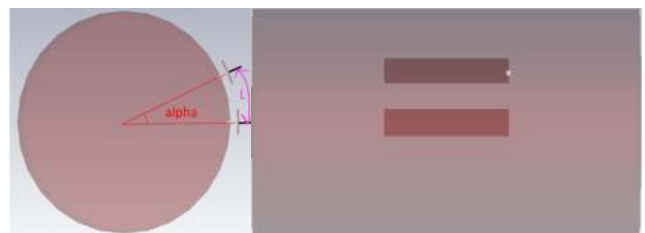

**FIGURE 4.** Model of the two parallel conformal rectangular microstrip antennas over the cylindrical implant: front view (left), side view (right). The white spot on the right side of the upper radiator corresponds to the probe.

The complex scattering matrix has been computed and the mutual impedance  $Z_{21}$  has been evaluated for different rotation angles  $\alpha$ , in the interval from  $\alpha_{min} = 25^\circ$  to  $\alpha_{max} = 180^\circ$  with a step of  $\Delta\alpha = 5^\circ$ . The corresponding results are reported in Fig. 5.

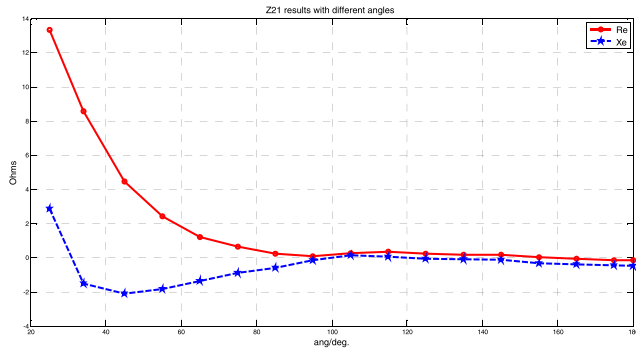


**FIGURE 5.** Real and imaginary part of the mutual impedance between the two conformal rectangular microstrip antennas for different rotation angles.

The data in Fig. 5 indicates that the coupling has an oscillatory behavior and presents a strong reduction while the distance between the antennas increases, similar to what happens for the planar case [27].

However, since the active input impedance  $Z_{inp}$  of the single element is influenced by the self-impedance of the two radiators  $Z_{11}$  and  $Z_{22}$  and by the mutual coupling  $Z_m$  according to

$$Z_{inp} = Z_{11} - \frac{Z_m^2}{Z_{22}}$$

for small angles the large coupling can have a significant effect. In order to reduce this effect, in the following section three methods for the reduction of mutual coupling are proposed and analyzed.

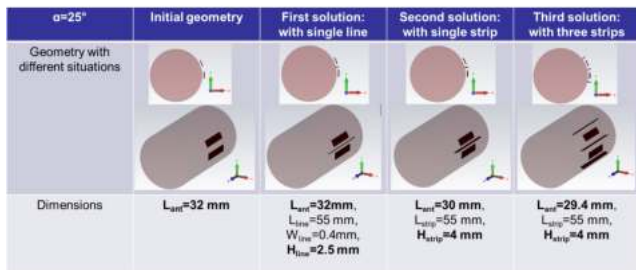


**FIGURE 6.** Three methods to reduce mutual coupling between the two antennas: first method (top), second method (middle), third method (bottom). For each case: front view (left), side view (right).

## V. REDUCTION OF THE MUTUAL COUPLING

Three methods, illustrated in Fig. 6, are investigated in this section in order to reduce mutual coupling between the two parallel antennas. First method is to introduce a grounded line between the two antennas. Second method is to introduce a grounded metallic strip between the two antennas. In the third


method this configuration is further extended by adding two more grounded strips at the two sides of the array.

In the first method, the material of the line is the same as of the implant and antennas. Its width has been chosen to be equal to 0.4 mm. Its height has been chosen to be equal to 2.5 mm which is the sum of the thickness of the first PDMS layer and the thickness of the antenna, i.e.  $th_{PDMS} + th_{met}$ . Its length has been chosen to avoid resonance; the value of 55 mm has been used in the following simulations performed in the angular interval of  $25^\circ$  to  $90^\circ$ . The two ends of the line are connected to the implant by two metallic cylinders. In the second method, the length of the strip is the same as the line of the first method while the height has been chosen to be equal to 4 mm, which is equal to the total thickness of the two PDMS layers. In the third method, all the three strips have the same dimensions as in the second method.

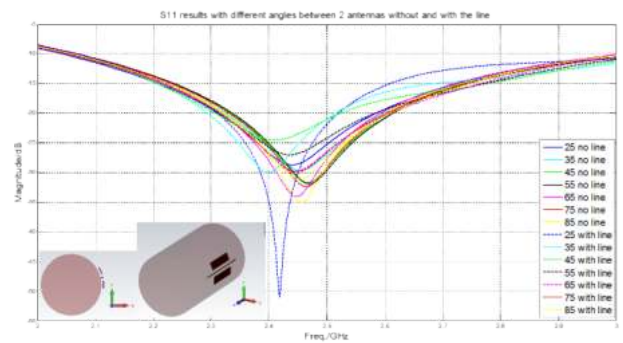

**FIGURE 7.** Input reflection coefficients for the first method (dotted lines) and for the initial case with no mutual coupling reduction (solid lines).

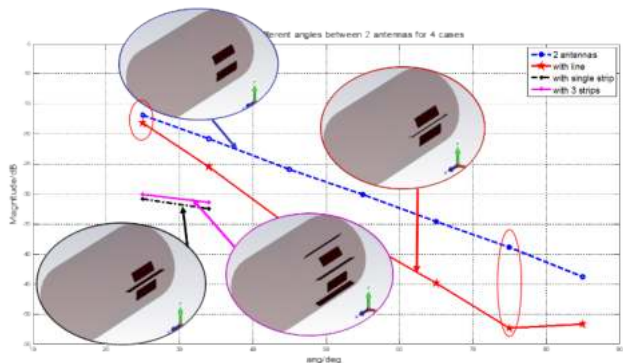Input reflection coefficients obtained for the first method (with a line) are compared with the initial case (without the line) in Fig. 7. As angle changes, the resonant frequency has a small shift because the mutual coupling changes with angle of rotation  $\alpha$ . With the proposed line, the resonant frequency also shifts compared to the initial situation without the line.

















**FIGURE 8.** Transmission coefficients for four cases: initial configuration and three mutual coupling reduction methods in Fig. 6.

The scattering matrix transmission coefficient magnitudes for the four analyzed cases in the angular interval from  $25^\circ$  to  $90^\circ$  are compared in Fig. 8. It can be observed that all



**TABLE 3.** Comparison of four cases for  $\alpha = 25^\circ$ : initial geometry, with single line, with single strip and with three strips.

$\alpha=25^\circ$	Initial case (no reduction)	First method	Second method	Third method
E field 				
Surface current 				
Radiation pattern				
Directivity (dBi)	6.159	6.590	5.828	6.567
Gain (dB)	-12.13	-12.26	-12.12	-11.03
Rad. efficiency (dB)	-18.32	-18.85	-17.95	-17.6
Total solver time	5 h, 43 m, 58 s	8 h, 21 m, 33 s	7 h, 54 m, 52 s	10 h, 34 m, 15 s


three methods can reduce mutual coupling by different levels. With the first method, the maximum coupling reduction is about 7 dB at  $75^\circ$  but for small angles mutual coupling reduction is not significant. With the second and third methods, reasonable mutual coupling reduction of about 13-14 dB can be achieved even for small angles. Consequently, the effect on the detuning is smaller, and the resulting reflection coefficients are closer to that of the single element in the stand-alone case.

In the following discussion, the effects of the proposed methods on the radiation performances are analyzed for the separation angle of  $25^\circ$ . Moreover, a broadside configuration has been considered, i.e., where the phase difference between the feeding signals of the two antennas is equal to zero. Table 2 compares the results for four cases considered before. For the sake of completeness, in Fig. 9 the same quantities, as reported in the Tab. 3, but for the single element are reported.

The first method leads to highest directivity, i.e., 6.59 dBi, but low efficiency, i.e.,  $-18.85$  dB. With second method, the efficiency increases, nevertheless the directivity is the lowest one among the three methods. Even though the third method takes the longest simulation time, its gain, radiation efficiency and directivity all demonstrate a significant improvement compared to the initial configuration. These figures are to be compared with the directivity of the single element, i.e. 4.35 dBi (See Fig. 9).

Comparing all the results, one can conclude that the most suitable solution is the third one, which can produce 13 dB reduction in mutual coupling. Moreover, it increases directivity by 0.4 dBi, gain by 1.1 dB and radiation efficiency by 0.9 dB. In situations where implementation of three strips is not practical, the second method may be acceptable as it also leads to good reduction in mutual coupling.

Furthermore, it can be observed that the pointing angle in the plane containing the symmetry axis of the structure

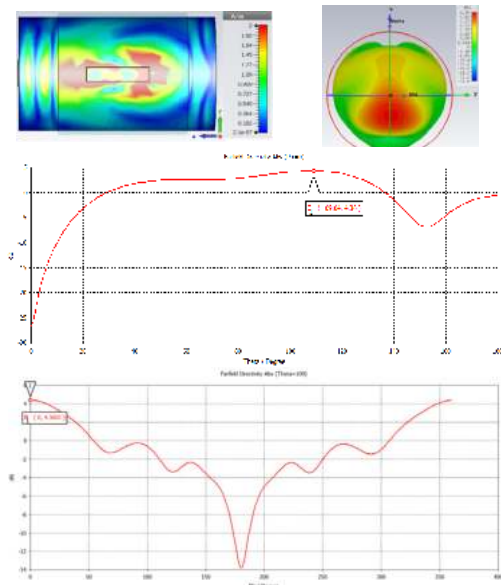

**FIGURE 9.** Surface current (top left) and 3D radiation pattern (top right) of the single antenna. xOz (middle) and xOy (bottom).

is varying. It is quite different with respect to the direction of the maximum radiation of the single antenna (see Fig. 9). As the mutual coupling reduces, the direction of the maximum radiation is closer to that of the single element.

## VI. CONCLUSIONS

Three solutions to reduce mutual coupling between two implanted microstrip antennas has been proposed. The extent of mutual coupling reduction has been quantified, and the best solutions have been identified. That is the insertion of a grounded, non-resonant, metallic strip halfway between the radiators and two additional strips on the two sides of the array. It was numerically verified that the reduced coupling manifests in higher gain and radiation efficiency, as expected. The coupling also influences the current distribution on the single radiators that in turn reflects in the tilted pointing angle of the two-element array. As the coupling reduces, the radiation pattern in the E-plane of the antenna is similar to the single element.

The proposed solution is feasible: in some cases following an injury, piece of a bone has to be replaced by an implant. When this occurs, instead of implanting a bare metallic cylinder (of bio-metal), the proposed geometry, i.e. bare cylinder equipped with the antenna(s) could be considered. The inside of the metallic cylinder could also host the necessary electronic part (signal generator, sensors, etc.).

## REFERENCES

- [1] M. S. Islam, K. P. Esselle, D. Bull, and P. M. Pilowsky, "Converting a wireless biotelemetry system to an implantable system through antenna redesign," *IEEE Trans. Microw. Theory Techn.*, vol. 62, no. 9, pp. 1890–1897, Sep. 2014.
- [2] Y. Zhao, R. Rennaker, C. Hutchens, and T. S. Ibrahim, "Simulation of implantable miniaturized antenna for brain machine interface applications," in *Proc. Adv. CEM Appl. IIACES conf.*, Columbus, OH, USA, 2012, pp. 1–6.
- [3] M. A. Shokry and A. M. M. A. Allam, "Implanted antenna in brain," in *Proc. IEEE Antennas Propag. Conf. (LAPC)*, Loughborough, U.K., Nov. 2013, pp. 630–633.
- [4] W. Xia, K. Saito, M. Takahashi, and K. Ito, "Performances of an implanted cavity slot antenna embedded in the human arm," *IEEE Trans. Antennas Propag.*, vol. 57, no. 4, pp. 894–899, Apr. 2009.
- [5] R. Alrawashdeh, Y. Huang, and A. A. B. Sajak, "A flexible loop antenna for biomedical bone implants," in *Proc. 8th Eur. Conf. Antennas Propag. (EUCAP)*, The Hague, The Netherlands, Apr. 2014, pp. 861–864.
- [6] P. Zakavi, N. C. Karmakar, and I. Griggs, "Wireless orthopedic pin for bone healing and growth: Antenna development," *IEEE Trans. Antennas Propag.*, vol. 58, no. 12, pp. 4069–4074, Dec. 2010.
- [7] Y. Ge, K. P. Esselle, and T. S. Bird, "E-shaped patch antennas for high-speed wireless networks," *IEEE Trans. Antennas Propag.*, vol. 52, no. 12, pp. 3213–3219, Dec. 2004.
- [8] H. Wang, D. Fang, and P. Ge, "Mutual coupling reduction between two conformal microstrip patch antennas," in *Proc. 5th Asia-Pacific Conf. Environ. Electromagn. (CEEM)*, Xi'an, China, Sep. 2009, pp. 176–179.
- [9] A. A. L. Neyestanak, F. Jolani, and M. Dadgarpour, "Mutual coupling reduction between two microstrip patch antennas," in *Proc. Electr. Comput. Eng.*, 2008, pp. 739–742.
- [10] A. Diallo, C. Luxey, P. L. Thuc, R. Staraj, and G. Kossias, "Study and reduction of the mutual coupling between two mobile phone PIFAs operating in the DCS 1800 and UMTS bands," *IEEE Trans. Antennas Propag.*, vol. 54, no. 11, pp. 3063–3074, Nov. 2006.
- [11] M. Ezzat and C. S. Lee, "A simple optimization technique for reducing mutual coupling between two coupled antennas," in *Proc. IEEE Int. Symp. Antennas Propag. USNC/URSI Nat. Radio Sci. Meeting*, Vancouver, BC, Canada, Jul. 2015, pp. 430–431.
- [12] Y. Kawakami, T. Hori, M. Fujimoto, R. Yamaguchi, and K. Cho, "Mutual coupling reduction effects of EBG structure located on cylinder surface," in *Proc. Antennas Propag. Soc. Int. Symp. (APSURSI)*, Toronto, ON, Canada, Jul. 2010, pp. 1–4.
- [13] J. Acharjee, K. Mandal, S. K. Mandal, and P. P. Sarkar, "Mutual coupling reduction between microstrip patch antennas by using a string of H-shaped DGS," in *Proc. Int. Conf. Microelectron. Comput. Commun. (MicroCom)*, Durgapur, India, Jan. 2016, pp. 1–3.
- [14] A. M. Abdalla, M. A. Abdelreheem, H. M. Abdegelel, and M. A. Ali, "Surface wave and mutual coupling reduction between two element array MIMO antenna," in *Proc. Antennas Propag. Soc. Int. Symp. (APSURSI)*, Lake Buena Vista, FL, USA, Jul. 2013, pp. 178–179.
- [15] I. C. Alagić, N. Gubelj, M. Rakin, Z. Cvijović, and Z. Gerić, "Microstructural morphology effects on fracture resistance and crack tip strain distribution in Ti-6Al-4V alloy for orthopedic implants," *Mater. Design*, vol. 53, pp. 870–880, Sep. 2014.
- [16] M. Wen, C. Wen, P. Hodgson, and Y. Li, "Fabrication of Ti-Nb-Ag alloy via powder metallurgy for biomedical applications," *Mater. Design*, vol. 56, pp. 629–634, Apr. 2014.
- [17] R. Kondo, N. Nomura, Suyalatu, Y. Tsutsumi, H. Doi, and T. Hanawa, "Microstructure and mechanical properties of as-cast Zr-Nb alloys," *Acta Biomater.*, vol. 7, pp. 4278–4284, Apr. 2011.
- [18] Suyalatu, R. Kondo, Y. Tsutsumi, H. Doi, N. Nomura, and T. Hanawa, "Effects of phase constitution on magnetic susceptibility and mechanical properties of Zr-rich Zr-Mo alloys," *Acta Biomater.*, vol. 7, pp. 4259–4266, Apr. 2011. [Online]. Available: <http://www.sciencedirect.com/science/article/pii/S1742706111003059>
- [19] L. D. Zardiackas, D. W. Mitchell, and J. A. Disegi, "Medical applications of titanium and its alloys," in *The Material and Biological Issues*, S. A. Brown and J. E. Lemons, Ed. West Conshohocken, PA, USA: ASTM Int., 1996, pp. 60–75.
- [20] I. Peter, L. Matekovits, and K. P. Esselle, "Metal-based materials for the development of implanted bio-devices," in *Proc. IEEE Int. Workshop Antenna Technol. (IWAT)*, Cocoa Beach, FL, USA, Feb./Mar. 2016, pp. 135–137.
- [21] M. Takahashi, M. Kikuchi, and O. Okuno, "Grindability of dental cast Ti-Zr alloys," *Mater. Trans.*, vol. 50, pp. 859–863, Apr. 2009.
- [22] I. Peter and M. Rosso, "Study of Ti-enriched CoCrMo alloy for dental application," *IEEE Access*, vol. 3, pp. 73–80, Jan. 2015.
- [23] W. F. Ho, C. P. Ju, and J. H. C. Lin, "Structure and properties of cast binary Ti-Mo alloys," *Biomaterials*, vol. 20, pp. 2115–2122, Apr. 1999.
- [24] W.-F. Ho, "A comparison of tensile properties and corrosion behavior of cast Ti-7.5 Mo with c.p. Ti, Ti-15 Mo and Ti-6 Al-4 V alloys," *J. Alloys Compounds*, vol. 464, nos. 1–2, pp. 580–583, 2008.

- [25] M. Nicoara, A. Raduta, R. Parthiban, C. Locovei, J. Eckert, and M. Stoica, "Low Young's modulus Ti-based porous bulk glassy alloy without cytotoxic elements," *Acta Biomater.*, vol. 36, pp. 323–331, Apr. 2016.
- [26] C. Ojeda, V. Chuman, A. Arriola, and M. Peña, "Microthread influence on strain-energy-based bone remodelling model," in *Proc. World Conf. Regenerative Med.*, Leipzig, Germany, Oct. 2015, pp. 1–6.
- [27] J. D. Kraus, *Antennas*. New York, NY, USA: McGraw-Hill, 1950.



**LADISLAU MATEKOVITS** (M'94–SM'11) received the degree in electronic engineering from the Institutul Politehnic din București, București, Romania, and the Ph.D. degree (Dottorato di Ricerca) in electronic engineering from the Politecnico di Torino, Torino, Italy, in 1992 and 1995, respectively. Since 1995, he has been with the Department of Electronics and Telecommunications, Politecnico di Torino, first with a Post-Doctoral Fellowship, and then as a Research Assistant. In 2005, he was Visiting Scientist with the Antennas and Scattering Department, Fraunhofer Institute, Wachtberg, Germany. He joined the Department of Electronics and Telecommunications as an Assistant Professor in 2002 and was appointed as a Senior Assistant Professor in 2005 and an Associate Professor in 2014, respectively. In 2009, for two years, he was a Marie Curie Fellow with Macquarie University, Sydney, NSW, Australia, where in 2013 he also held a visiting academic position and in 2014 was appointed as an Honorary Fellow. His main research activities concern numerical analysis of printed antennas and in particular development of new, numerically efficient full-wave techniques to analyze large arrays, optimization techniques, and active and passive metamaterials. Material parameter retrieval of these structures by inverse methods and different optimization techniques has also been considered. In the last years, bio-electromagnetic aspects have also been contemplated, as for example design of implantable antennas or development of nano-antennas, for example, for drug delivery applications.

He has authored almost 300 papers, including over 60 journal contributions, and delivered seminars on these topics all around the world: Europe, USA (AFRL/MIT-Boston), Australia, and China. He has been invited to serve as a Research Grant Assessor for government funding calls and as an International Expert in Ph.D. thesis evaluation by several universities from Australia, India, and Spain.

Dr. Matekovits is recipient of various awards in international conferences, including the 1998 URSI Young Scientist Award, Thessaloniki, Greece, the Barzilai Award 1998 (Young Scientist Award, granted every two years by the Italian National Electromagnetic Group), and the Best AP2000 Oral Paper on Antennas, ESA-EUREL Millennium Conference on Antennas and Propagation, Davos, Switzerland.

He is a member of the Organizing Committee of the International Conference on Electromagnetics in Advanced Applications and technical program committees of several conferences. He has been the Assistant Chairman and the Publication Chairman of the European Microwave Week 2002, Milan, Italy, and the General Chair of the 11th International Conference on Body Area Networks (BodyNets) 2016. He serves as an Associate Editor of IEEE ACCESS and the IEEE ANTENNAS AND WIRELESS PROPAGATION LETTERS and a reviewer for different journals.



**JIE HUANG** received the B.A. degree in electrical engineering and automation from Luoyang Normal University, China, in 2014, and the M.A. degree in wireless system design from the Politecnico di Torino, Torino, Italy, in 2016, respectively. Her research interest is in printed antennas for UWB and medical applications.



**ILDIKO PETER** received the M.S. degree in biochemistry from the Università degli Studi di Torino in 1999 and the Ph.D. degree in material science and engineering from the Politecnico di Torino, Italy, in 2006. She is involved in the teaching activity of various Master's and Ph.D. level courses in the field of material science. In 2010 she was a Visiting Researcher with Macquarie University, Sydney, NSW, Australia. She has participated in various European and National projects being involved at both technical/research and administrative levels. She has co-authored over 100 publications and holds two granted patents. Her research interest is oriented to the development and characterization of light weight alloys by traditional and innovative techniques for automotive and aeronautical industries, the study of metallic materials for biomedical applications, the synthesis and characterization of innovative substrates for advanced electromagnetic applications, the study of Al and Mg alloys welding and development of coatings on light alloys and on steel substrate for high temperature applications. She has delivered various invited talks, and organized special sessions at several conferences. She is acting as a TPC Member of different international conferences and as a reviewer for several journals. She is the European Branch Director of the American Romania Academy. Since 2015, she has been serving as an Associate Editor of IEEE ACCESS.



**KARU P. ESSELLE** (M'92–SM'96–F'16) received the B.Sc. degree (Hons.) in electronic and telecommunication engineering from the University of Moratuwa, Sri Lanka, and the M.A.Sc. and Ph.D. degrees in electrical engineering from the University of Ottawa, Canada. He is currently a Professor of Electronic Engineering, Macquarie University, Sydney, one of the two directors of the WiMed Research Centre and the Past Associate Dean—Higher Degree Research of the Division of Information and Communication Sciences. He has also served as a member of the Dean's Advisory Council and the Division Executive from 2003 to 2008 and the Head of the Department several times. He was elevated to the IEEE Fellow grade for his contributions to resonance-based antennas. He is also a Fellow of Engineers Australia. He is also the Chair of the Board of management of Australian Antenna Measurement Facility, and the Elected Chair of the IEEE New South Wales (NSW) Section and the IEEE NSW AP/MTT Chapter, in 2016 and 2017, respectively. He directs the Centre for Collaboration in Electromagnetic and Antenna Engineering, and has been selected as one of the three new Distinguished Lecturers of the IEEE AP Society for 2017–2020. He is the first Australian AP Distinguished Lecturer (DL) in almost two decades, and the second Australian AP DL ever. When he was elected to the IEEE Antennas and Propagation Society Administrative Committee for a three year term in 2014, he became the only person residing in the Asia-Pacific Region (IEEE Region 10) to be elected to this highly competitive position over a period of at least six years from 2010 to 2015.

He has authored over 500 research publications and his papers have been cited almost 4,300 times. He is the first Australian antenna researcher ever to reach Google Scholar h-index of 30 and his current h-index is the highest among Australian antenna researchers when Google Scholar errors are corrected. Since 2002, his research team has been involved with research grants, contracts and Ph.D. scholarships worth over 15 million dollars. His research has been funded by many national and international organizations, including Australian Research Council, Intel, US Air Force, Cisco Systems and Hewlett-Packard, and Australian and Indian governments.



He has been invited to serve as an International Expert/Research Grant Assessor by several nationwide research funding bodies overseas, including The Netherlands, Canada, Finland, Hong Kong, Georgia, and Chile. He has been invited by Vice-Chancellors of Australian and overseas universities to assess applications for promotion to professorial levels. He has also been invited to assess grant applications submitted to Australia's most prestigious schemes, such as Australian Federation Fellowships and Australian Laureate Fellowships. He leads the Implantable Wireless Program of the WiMed Research Centre. In addition to the large number of invited conference speeches he has given, he has been an invited Keynote Speaker of IEEE workshops and conferences.

Dr. Esselle received the 2016 and 2012 Best Published Paper Awards from IESL NSW Chapter, the 2011 Outstanding Branch Counsellor Award from the IEEE Headquarters, USA, the 2009 Vice Chancellor's Award for Excellence in Higher Degree Research Supervision, and the 2004 Inaugural

Innovation Award for best invention disclosure. His mentees have received many fellowships, awards, and prizes for their research achievements; 36 international experts who examined the theses of his recent Ph.D. graduates ranked them in the top 5% or 10%.

He has provided expert assistance to more than a dozen companies, including Intel, Hewlett Packard Laboratory, USA, Cisco Systems, USA, Cochlear, Optus, ResMed, and Katherine-Werke, Germany. He is an Associate Editor of the IEEE TRANSACTIONS ON ANTENNAS AND PROPAGATION and IEEE ACCESS.

He is General Co-Chair of IEEE TENSYP 2018, the Technical Program Committee Co-Chair of ISAP 2015, APMC 2011, and TENCON 2013 and the Publicity Chair of ICEAA 2016, IWAT 2014, and APMC 2000. He is the Foundation Counsellor of the IEEE Student Branch at Macquarie University, and the Foundation Advisor of the IEEE MTT Chapter in Macquarie University.

...