

POLITECNICO DI TORINO  
Repository ISTITUZIONALE

An international trilateral comparison among the newest generations of digital and Josephson impedance bridges

*Original*

An international trilateral comparison among the newest generations of digital and Josephson impedance bridges / Ortolano, Massimo; Marzano, Martina; Overney, Frédéric; Eichenberger, Ali L.; Kucera, Jan; D'Elia, Vincenzo; Bartova, Lucie; Medved, Juan; Callegaro, Luca. - In: IEEE TRANSACTIONS ON INSTRUMENTATION AND MEASUREMENT. - ISSN 0018-9456. - ELETTRONICO. - 74:(2025), pp. 1-9. [10.1109/tim.2025.3541803]

*Availability:*

This version is available at: 11583/2997924 since: 2025-02-26T18:14:47Z

*Publisher:*

IEEE

*Published*

DOI:10.1109/tim.2025.3541803

*Terms of use:*

This article is made available under terms and conditions as specified in the corresponding bibliographic description in the repository

*Publisher copyright*

(Article begins on next page)

# An International Trilateral Comparison Among the Newest Generations of Digital and Josephson Impedance Bridges

Massimo Ortolano<sup>1</sup>, Martina Marzano<sup>2</sup>, Frédéric Overney<sup>3</sup>, *Member, IEEE*, Ali L. Eichenberger<sup>4</sup>, Jan Kucera<sup>5</sup>, Vincenzo D'Elia<sup>6</sup>, Lucie Bartova<sup>7</sup>, Juan Medved<sup>8</sup>, *Graduate Student Member, IEEE*, and Luca Callegaro<sup>9</sup>, *Member, IEEE*

**Abstract**—This work reports and thoroughly discusses the results of an onsite trilateral comparison between a dual Josephson impedance bridge developed by METAS and the electronic fully digital impedance bridges developed by CMI and INRIM-POLITO. The target accuracies of the bridges are at the level of  $10^{-9}$  to  $10^{-8}$  for the former and at the level of parts in  $10^7$  for the latter. The bridges were tested with  $R:R$  and  $R:C$  standards, with nominal magnitudes of 12.9 k $\Omega$ , and with a quantum Hall resistance standard, in conditions suitable for the primary direct realization of the impedance units ohm and farad from ac quantum Hall resistance standards or from ac/dc calculable transfer resistance standards calibrated against dc quantum Hall resistance standards. The results were fully compatible at the expected level of uncertainty for what concerns the magnitude ratio, but phase measurements with  $R:C$  standards showed some incompatibilities.

**Index Terms**—Bridge circuits, calibration, impedance measurement, Josephson effect, metrology.

## I. INTRODUCTION

IMPEDANCE bridges [1] of various constructions are used by national metrology institutes (NMIs) around the world to provide the traceability to the International System of Units (SI) of the units of impedance ohm, farad, and henry.

In recent years, there has been a progressive transition from traditional impedance bridges based on transformers or inductive voltage dividers to novel impedance bridges based

on electronic or Josephson arbitrary waveform synthesizers. This transition has been stimulated by the fact that contrary to transformer-based bridges, electronic fully digital impedance bridges (FDIBs) and dual Josephson impedance bridges (DJIBs) with relatively simple architectures are capable of directly comparing impedances across the whole complex plane and operating over a wide range of frequencies. For instance, these kinds of bridges can directly compare like impedances (e.g.  $R:R$  or  $C:C$ ) or unlike impedances (e.g.  $R:C$  or  $R:L$ ), determining both magnitude (modulus) and phase angle (argument) of the complex ratio. FDIBs are also relatively affordable, easy to operate, and transportable but less accurate than DJIBs. The target accuracies are at the level of  $10^{-9}$  to  $10^{-8}$  for DJIBs and at the level of parts in  $10^7$  for FDIBs. In the last decade, the transition from traditional bridges to FDIBs and DJIBs has been specifically promoted in Europe by a number of collaborating NMIs and universities through projects<sup>1</sup> funded by the European Association of National Metrology Institutes (EURAMET). Since the first prototypical FDIB [2], NMIs have been, thus, continually improving FDIBs and DJIBs such that these kinds of devices are currently mature enough for primary impedance metrology applications. Of particular interest is the application of FDIBs and DJIBs to the direct realization of the unit farad either from ac quantized Hall resistance (QHR) standards or from ac/dc calculable transfer resistance standards calibrated against dc QHR standards, thus avoiding the usage of complex transformer-based quadrature bridges.

However, the application of FDIBs and DJIBs to primary impedance metrology requires a careful assessment of their performances and their mutual compatibility at a number of relevant impedance ratios and frequencies. A first international comparison between FDIBs aimed at the calibration of secondary impedance standards was run from 2015 to 2018 [3]. For the assessment of FDIBs and DJIBs aimed at primary metrology applications, the Istituto Nazionale di Ricerca Metrologica (INRIM), Italy, the Federal Institute of Metrology

Received 27 October 2024; revised 20 December 2024; accepted 2 January 2025. Date of publication 13 February 2025; date of current version 27 February 2025. This work was supported in part by the Project CAPSTAN Quantum Electrical Italian National Capacitance Standard Funded by the Ministero dell'Università e della Ricerca (MUR) Progetti di Ricerca di Rilevante Interesse Nazionale (PRIN) Bando 2020 under Grant 2020A2M33J and in part by the Institutional Subsidy for Long-Term Conceptual Development of a Research Organization granted to the Czech Metrology Institute by the Ministry of Industry and Trade. The Associate Editor coordinating the review process was Dr. Yasutaka Amagai. (*Corresponding author: Massimo Ortolano.*)

Massimo Ortolano is with the Politecnico di Torino (POLITO), 10129 Turin, Italy (e-mail: massimo.ortolano@polito.it).

Martina Marzano, Vincenzo D'Elia, and Luca Callegaro are with the Istituto Nazionale di Ricerca Metrologica (INRIM), 10135 Turin, Italy.

Frédéric Overney and Ali L. Eichenberger are with the Federal Institute of Metrology METAS, CH-3003 Berne-Wabern, Switzerland.

Jan Kucera and Lucie Bartova are with the Czech Metrology Institute (CMI), 63800 Brno, Czech Republic.

Juan Medved is with INRIM, 10135 Turin, Italy, and also with POLITO, 10129 Turin, Italy.

Digital Object Identifier 10.1109/TIM.2025.3541803

<sup>1</sup>Namely, the projects AIM QuTE (2013–2016), *automated impedance metrology extending the quantum toolbox for electricity*, VersiCaL (2018–2021), *a versatile electrical impedance calibration laboratory based on digital impedance bridges*, and GIQS (2019–2022), *graphene impedance quantum standard*.

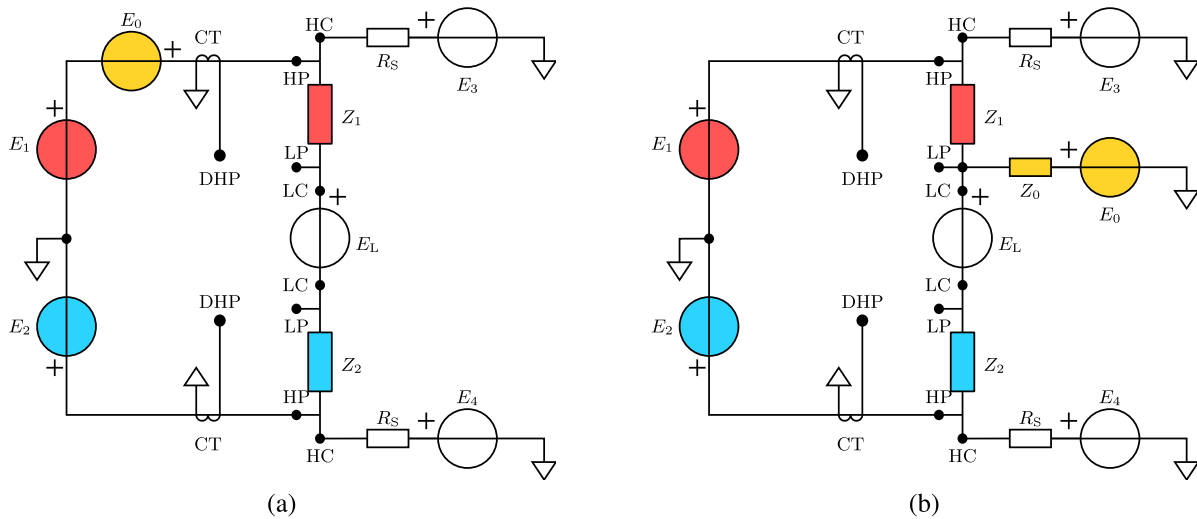


Fig. 1. Simplified principle schematics of the FDIBs and the DJIB used in the comparison. (a) CMI FDIB and METAS DJIB. (b) INRIM-POLITO FDIB. The measured impedances are  $Z_1$  and  $Z_2$  with terminal pairs labeled HC, HP, LP, and LC. The voltage sources  $E_1$  and  $E_2$  generate the reference voltage ratio  $E_1/E_2$  to which the impedance ratio  $Z_1/Z_2$  is compared. In the DJIB,  $E_1$  and  $E_2$  are the outputs of a dual Josephson arbitrary waveform synthesizer; in the FDIBs,  $E_1$  and  $E_2$  are two output channels of an electronic digital synthesizer. In both types of bridges, the auxiliary voltages  $E_0$ ,  $E_3$ ,  $E_4$ , and  $E_L$  are generated by an electronic synthesizer. In (a),  $E_0$  and  $E_L$  are injected by means of a step-down transformer (100:1 turns ratio); in (b),  $E_L$  is injected by means of a step-down transformer (200:1 turns ratio), and  $Z_0$  is a 1 or 10-pF capacitance standard. The bridge balances are checked at the terminal pairs LP and DHP. The transformer CT detects the currents through the HP terminal pairs.

(METAS), Switzerland, the Physikalisch-Technische Bundesanstalt (PTB), Germany, and the Politecnico di Torino (POLITO), Italy, started in 2020 the project EURAMET TC-EM 1501, *technical assessment of novel digital impedance bridges* [4]. The project is being coordinated by INRIM, and the Czech Metrology Institute (CMI), Czech Republic, joined it at the end of 2023. A first round of comparisons within this project took place from September to November 2021 when the INRIM-POLITO FDIB was moved to Braunschweig to be compared with the PTB DJIB. The results of this first round were published in [5]. A second round of comparisons took place in 2023 in Bern, where the INRIM-POLITO FDIB (from mid-October to December) and the CMI FDIB (one week in mid-October) were moved to and compared with the METAS DJIB. This work fully reports on these new results, a selection of which was first summarily reported in [6].

The plan is given as follows. Sections II and III briefly describe the impedance bridges and the standards involved in the comparison. Section IV presents the main results of the trilateral comparison and discusses some technical difficulties that arose during the comparison. The Appendix presents some additional results that were obtained during the subsequent period in which only the INRIM-POLITO FDIB remained at METAS.

## II. PARTICIPATING IMPEDANCE BRIDGES

An impedance bridge determines the complex impedance ratio  $Z_1/Z_2$  of two impedances  $Z_1$  and  $Z_2$ . The simplified principle schematics of the DJIB and the two FDIBs participating in this work are represented in Fig. 1 in a comparative way. The two impedance standards are defined as four-terminal-pair (4TP) standards [7] with the terminal pairs labeled HC (high current), HP (high potential), LP (low potential), and LC (low current). The DJIB and the two FDIBs are *sourcing bridges* [8], in which the impedance ratio is determined from

a reference voltage ratio generated by the channels  $E_1$  and  $E_2$  of a multiphase source. In the DJIB, the source is a dual Josephson arbitrary waveform synthesizer (JAWS); in the FDIBs, the source is an electronic digital synthesizer. The injection channel  $E_0$  in Fig. 1(a) and the injection arm  $E_0$ - $Z_0$  in Fig. 1(b) are used to improve the resolution and the accuracy of the balance. The 4TP definition of the impedances is realized by the auxiliary channels  $E_3$ ,  $E_4$ , and  $E_L$ , the resistors  $R_S$ , and the current detection transformer CT. A bridge is balanced when both the mean (main balance) and the difference (Kelvin balance) of the LP voltages are zero, and when the HP currents, as measured at the detection terminal pairs DHP are zero (current balances). To compensate for possible asymmetries in the bridge networks, the measurements are performed in two successive configurations, typically labeled *forward* and *reverse*, differing by the exchange of the impedances.

Fig. 2 shows a picture of the three bridges in the METAS laboratory.

The CMI FDIB, shown schematically in Fig. 1(a), is based on the reconfigurable bridge [11], where the reference ratio of the bridge is formed by the ultrastable two-channel source SWG [12]. The 4TP definition of the impedances under comparison is fulfilled by means of additional fully synchronized SWG sources and an injection circuit. In the 1:1 ratio mode, a two-step measurement is performed, where rebalancing in the second step is done with an additional injection circuit situated in one of the potential arms [ $E_0$  in Fig. 1(a)]. The full automation of the bridge balancing with one lock-in amplifier and the reversing of source channels is performed with the second generation of coaxial switches based on [13]. The high stability of channel outputs and the low crosstalk between the two reference channels (both around  $10 \text{ nV V}^{-1}$ ) ensure the negligible influence of channel swapping and phase rotation of one channel on the output voltage of the second one.

TABLE I  
LIST OF THE RESISTANCE ( $R$ ) AND CAPACITANCE ( $C$ ) STANDARDS EMPLOYED IN THE COMPARISON

| Impedance label | Serial number     | Nominal value        | Description   |
|-----------------|-------------------|----------------------|---|
| $R_1$           | G1_1132           | 12 906.4035 $\Omega$ | NL Engineering UK Gibbings-type calculable quadrifilar resistance standard    |
| $R_2$           | G2_1137           | 12 906.4035 $\Omega$ | NL Engineering UK Gibbings-type calculable quadrifilar resistance standard    |
| $R_{QHR}$       | G1511_41_96       | 12 906.4037 $\Omega$ | PTB graphene AC QHR standard mounted on a METAS TO-8 holder [9]               |
| $C_1$           | 10nF_SUT_METAS    | 10 nF                | GUM-SUT construction with Murata GRM31 series COG SMD capacitor [10]          |
| $C_2$           | INRIM_01-2021_8nF | 8 nF                 | INRIM construction with GenRad 1409 capacitance standard (1 nF + 2 nF + 5 nF) |



Fig. 2. METAS laboratory with some of the authors and the three installed bridges: from left to right, METAS DJIB, CMI FDIB, and INRIM-POLITO FDIB.

The INRIM-POLITO FDIB, shown schematically in Fig. 1(b), is optimized for 1:1 ratio magnitudes and is based on a polyphase digital source [14] with seven independently adjustable channels. Two channels provide  $E_1$  and  $E_2$ , generating the main voltage ratio: one channel provides the auxiliary injection  $E_0$ , and the other channels are used to implement the 4TP definition of the impedances. The main, Kelvin, and current balances are detected by a lock-in amplifier, which is automatically switched across the various detection terminal pairs. A single complete measurement requires about 10 min to 15 min. The operating principle of the INRIM-POLITO FDIB, its balancing procedure, and its implementation without the full automation are described in detail in [15]. The bridge is now fully automated, and a number of improvements in the balancing procedure have been implemented.

The METAS DJIB, shown schematically in Fig. 1(a), relies on the reference voltages  $E_1$  and  $E_2$  generated by a dual JAWS system developed by the National Institute of Standards and Technology (NIST), Boulder, CO, USA. It consists of two JAWS chips mounted in separate probes, both cooled to 4.2 K within the same LHe dewar. Each JAWS chip comprises four arrays, totaling 51 240 Josephson junctions (JJs) [16]. While each JAWS chip can generate an rms voltage up to 1 V at a pulse repetition of 14.4 GHz, the system operates in a “zero-compensation” mode [17], limiting the maximum rms voltage to 0.3 V. The dual JAWS system provides reference voltages to a four-terminal-pair digitally assisted bridge developed by METAS [18]. This bridge allows accurate measurement of impedance ratios from 1:10 to 10:1 at frequencies ranging

from less than 1 kHz to 80 kHz. The bridge is fully automated. The balancing and measurement procedure performed at a given frequency typically requires about 7 min. To compensate for the loading effect of the cables from the JAWS chip output inside the LHe dewar and the bridge in the laboratory, the balancing and measurement procedure must be repeated with the positions of the two impedance standards inverted. Therefore, the time required to perform a complete measurement cycle at a given frequency is about 14–16 min. For a comprehensive understanding of the DJIB, including its detailed working principle, balancing procedure, and performance metrics, refer to [19].

Before the international comparisons at PTB and METAS, the three bridges described in this section were also compared locally against the previous generation of transformer-ratio impedance bridges and reference standards operating at the respective institutions. The comparisons with the transformer-ratio bridges were described in [11], [15], [19], and [20].

### III. COMPARED STANDARDS

The impedance bridges were compared with  $R:R$  and  $R:C$  standards at ratio magnitudes close to 1:1 (typically within few parts in  $10^5$ ). Table I and Fig. 3 list the standards employed in the comparison.

All room-temperature standards are temperature-controlled. A detailed description of the 10 nF capacitance standard 10nF\_SUT\_METAS is given in [10]; a description and a characterization of the graphene ac QHR standard are given in [9]. This device was operated in a liquid helium cryostat at a temperature of 4.2 K and at magnetic flux densities ranging from about 8 T to 10 T.

The standards  $R_1$ ,  $R_2$ ,  $C_1$ , and  $C_2$  are defined as 4TP impedances. The ac QHR standard is defined as a 4TP impedance at two star points at the top of the cryostat, with triple connections [21] from the ac QHR standard to the star points. Four active current equalizers ensure the current equalization of the triple connections. The bridges were connected to the two standards under measurement with equal-length cables such that the cable effect is compensated by the ratio measurement [21]. The cable lengths were about 2 m and 4 m, depending on the position of the bridges in the laboratory with respect to the standards.

The matrix of Table II lists the impedance pairs that were measured during the comparison, with the measuring bridges and the measurement frequencies for each pair. For  $R:C$  measurements, the frequency  $f$  is such that  $2\pi f RC \approx 1$ . The



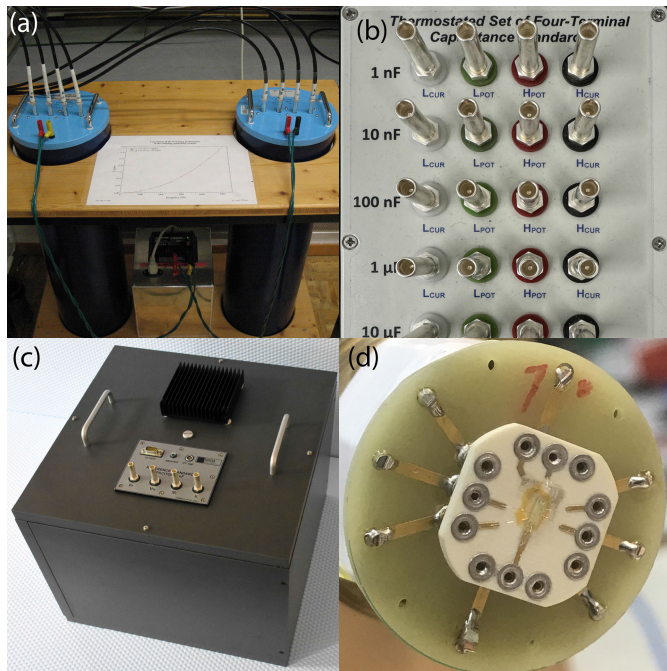


Fig. 3. Pictures of the impedance standards employed in the comparison. (a)  $R_1$  and  $R_2$ . (b)  $C_1$ . (c)  $C_2$ . (d)  $R_{QHR}$ .

TABLE II

LIST OF THE IMPEDANCE STANDARDS PAIRS MEASURED DURING THE COMPARISON. FOR EACH PAIR, THE MEASURING BRIDGES AND THE MEASUREMENT FREQUENCIES ARE ALSO LISTED

|       | $R_1$   | $R_{QHR}$                                   |
|-------|---|---|
| $R_1$ |   | CMI<br>INRIM-POLITO<br>METAS<br>1233.147 Hz |
| $R_2$ | CMI<br>INRIM-POLITO<br>METAS<br>1000 Hz, 1233.147 Hz, 5000 Hz |   |
| $C_1$ | CMI<br>INRIM-POLITO<br>METAS<br>1233.147 Hz                   | CMI<br>INRIM-POLITO<br>METAS<br>1233.147 Hz |
| $C_2$ | INRIM-POLITO<br>METAS<br>1541.434 Hz                          |   |

frequency 1233.147 Hz used for the measurements with  $C_1$  is also of practical interest because it is close to one of those typically adopted for the representation of the farad and in international comparisons. The frequency 1541.434 Hz used for the measurements with  $C_2$  is close to the one currently adopted at INRIM in the traceability chain of the farad [15]. During the measurements of the pair  $C_1:R_1$ , a General Radio 1422-CD variable air capacitor was connected in parallel to  $R_1$ , across the terminal pairs HC and LP to avoid increasing the cable correction, and set to a nominal value of 1.464 pF to adjust the phase angle to a value close to  $-90^\circ$ .

#### IV. RESULTS AND DISCUSSION

In this section, we present the results of the comparison. We have chosen to display the results in the form of plots to better cover extended periods of time and highlight potential drifts. In all plots, the uncertainty bars represent standard uncertainties with coverage factor  $k = 1$ .

The symbols  $R_1$ ,  $R_2$ ,  $R_{QHR}$ ,  $C_1$ , and  $C_2$  denote both the standards (the objects) and their primary parameters, resistance, or capacitance. The symbols  $Z(R_1)$ ,  $Z(R_2)$ ,  $Z(R_{QHR})$ ,  $Z(C_1)$ , and  $Z(C_2)$  denote the associated complex impedances. Where convenient, the impedances are represented with a parallel equivalent model, such that  $Z(R_n) = R_n/(1-j2\pi f\tau_n)$ , with  $\tau_n$  being the resistor time constant and  $n = 1, 2$ , and  $Z(C_n) = 1/(G_n + j2\pi fC_n)$ , with  $G_n$  being the capacitor parallel conductance.

The plots in Fig. 4 show the results for the  $C_1:R_1$  ratio measurements at 1233.147 Hz with all three bridges. It can be observed from Fig. 4(a) that the results for the magnitude ratio  $|Z(C_1)/Z(R_1)|$  are generally compatible, for most measurements within the standard uncertainties, and for all measurements within the expanded uncertainties with coverage factor  $k = 2$ . However, Fig. 4(b) shows incompatibility between the measurements of the phase,  $\arg Z(C_1)/Z(R_1) = \arg Z(C_1) - \arg Z(R_1)$ . The discrepancies between the results of the INRIM-POLITO FDIB from those of the METAS DJIB decrease after October 29, date marked by the vertical dashed line. Before this date, the impedances in the INRIM-POLITO FDIB were exchanged from the forward to the reverse configurations only at the terminal pairs HP and HC, leaving the terminal pairs LP and LC unexchanged; as a result, the asymmetry of the Kelvin arm containing  $E_L$  was not compensated, and this caused a significant phase deviation. It was then decided to exchange the impedances at all terminal pairs, and the phase deviation has been reduced from October 29. There remains, however, a residual incompatibility between the phase measurements, which is likely due to an uncompensated asymmetry in the INRIM-POLITO FDIB between the forward and reverse configurations. This uncompensated asymmetry may be caused by either the source crosstalk (see [8]: this is accounted for in the uncertainty budget, but it might have been underestimated) or the potentially limited efficiency of the passive current equalizers employed in the network of the INRIM-POLITO FDIB. In fact, about the latter cause of asymmetry, common-mode current measurements in the INRIM-POLITO FDIB yielded excessively high values in some branches of the bridge network for certain arrangements of the bridge equipment in the laboratory, with values changing from the forward to the reverse configurations, and this suggests that there were measuring conditions in which the current equalizers were not enough effective. Similar behavior was observed with the CMI FDIB on later measurements [see Fig. 5(b) and (d)], where the phase deviation of the measurement was significantly lowered when all terminal pairs of  $C_1$  and  $R_1$  were swapped or even when only the reference voltage sources  $E_1$  and  $E_2$  were swapped. Additional measurements of crosstalk between sources  $E_1$  and  $E_2$  in the CMI FDIB demonstrated negligible crosstalk effects (on the level of  $10^{-9}$ ) [22]; thus, the current equalization in the

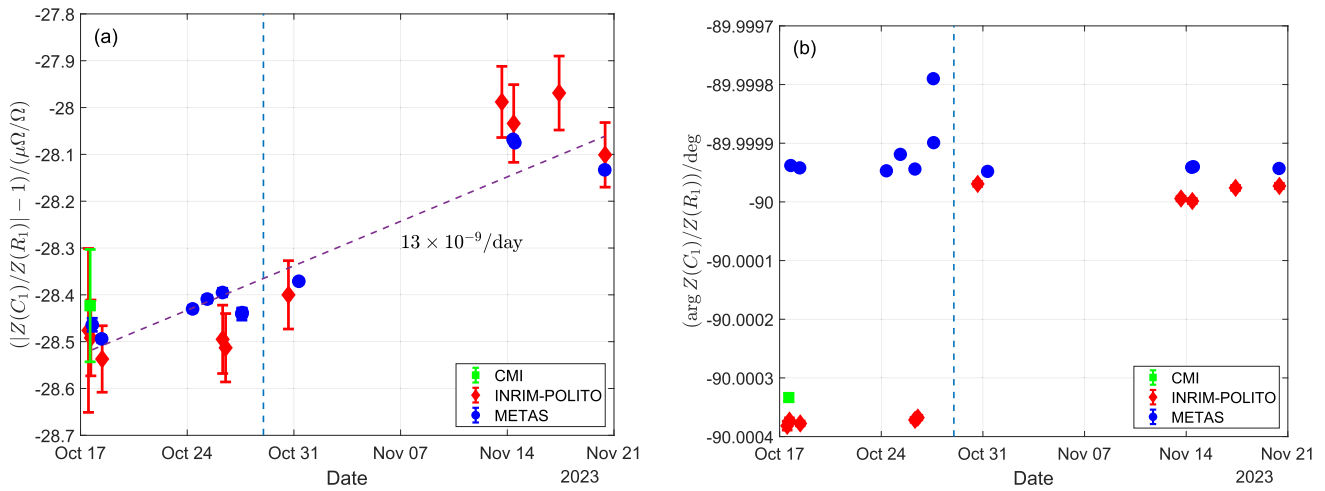


Fig. 4. Measurement results for the  $C_1:R_1$  ratio at 1233.147 Hz. (a) Deviation from the unit of the impedance magnitude ratio,  $|Z(C_1)/Z(R_1)|$ . (b) Angle of the impedance ratio,  $\arg Z(C_1)/Z(R_1)$ . The uncertainty bars represent the standard uncertainties with coverage factor  $k = 1$ . The vertical dashed line in plots (a) and (b) marks October 29, when, afterward, the impedances in the INRIM-POLITO FDIB were fully exchanged between the forward and reverse configurations. The oblique dashed line in plot (a) represents the least-square fit of the METAS DJIB measurements, indicating a relative drift coefficient of  $C_1$  of about  $13 \times 10^{-9} \text{ d}^{-1}$ .

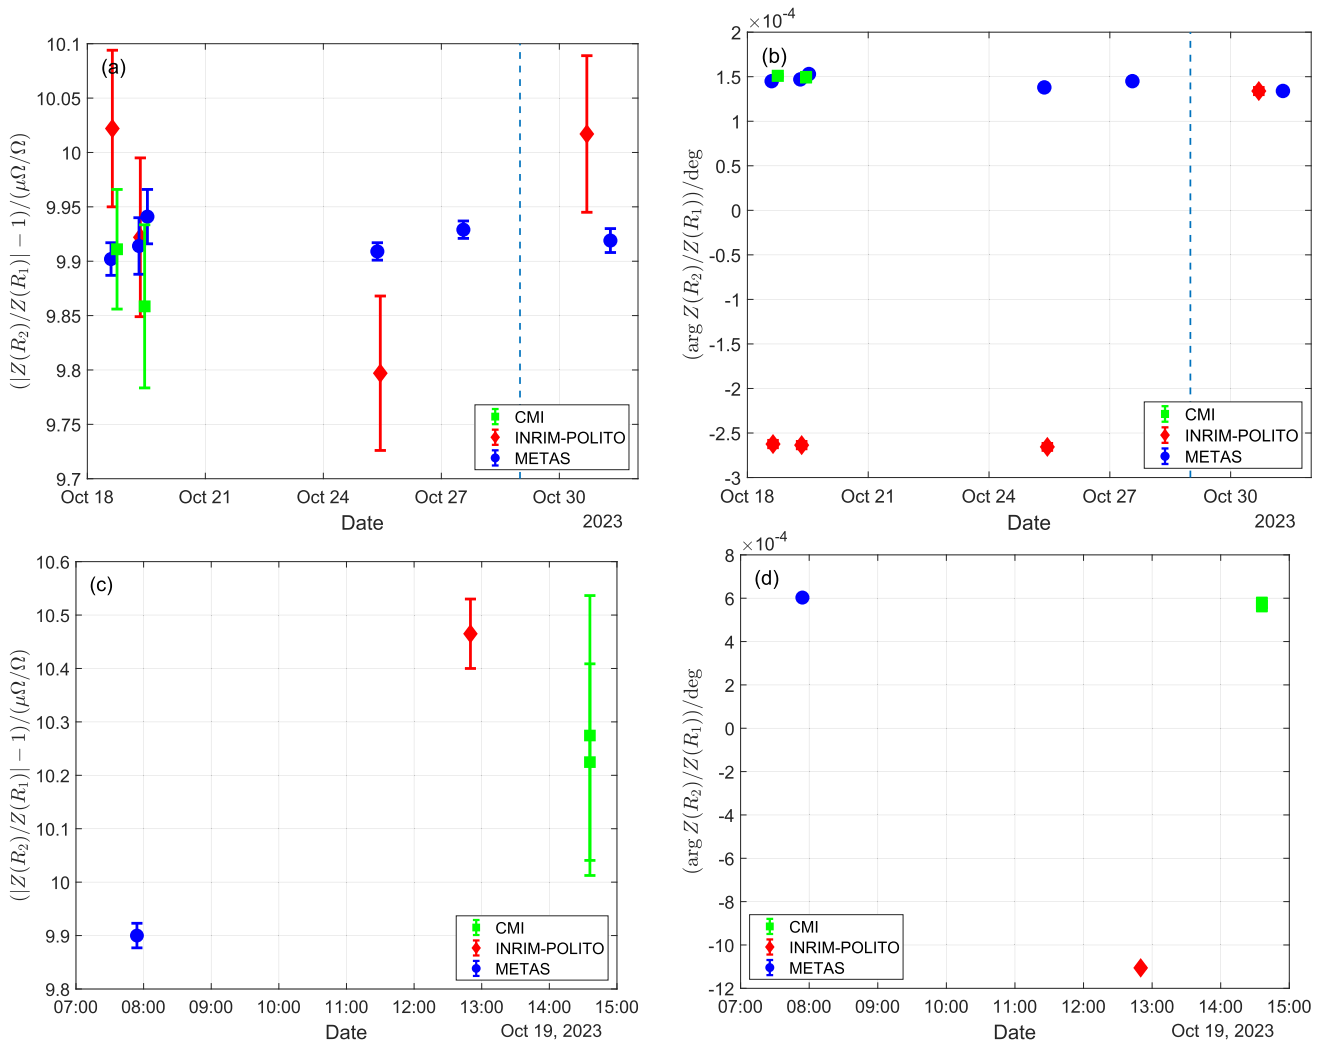


Fig. 5. Measurement results for the  $R_2:R_1$  ratio. (a) and (c) Deviation from the unit of the impedance magnitude ratio,  $|Z(R_2)/Z(R_1)|$ . (b) and (d) Angle of the impedance ratio,  $\arg Z(R_2)/Z(R_1)$ . (a) and (b) Measurements at 1233.147 Hz. (c) and (d) Measurements at 5000 Hz. The uncertainty bars represent the standard uncertainties with coverage factor  $k = 1$ . The vertical dashed line in plots (a) and (b) marks October 29, as in Fig. 4.

network is supposed to be the source of asymmetry. Further investigations on these effects will be performed in the future.

Fig. 4(a) reports also the relative drift of  $|Z(C_1)/Z(R_1)|$ , which virtually coincides with the drift of  $C_1$ . The oblique

TABLE III  
INRIM-POLITO FDIB MEASUREMENT RESULTS FOR THE  $R_2:R_1$   
RATIO (SEE TEXT FOR DETAILS)

| Date        | $f$      | $\frac{(R_2 - R_2^{\text{REF}})/R_2^{\text{REF}}}{n\Omega/\Omega}$ | $\frac{\tau_2 - \tau_2^{\text{REF}}}{\text{ps}}$ | Repetitions | Measurement time |
|-------------|----------|--|--|-------------|------------------|
| 22 Nov 2023 | 1000.000 | 35(75)   | 13(11)   | 6           | 48 min           |
| 22 Nov 2023 | 5000.000 | 57(140)  | 13(5)  | 8           | 95 min           |
| 23 Nov 2023 | 1008.704 | 61(72)   | 5(11)  | 8           | 65 min           |
| 23 Nov 2023 | 4983.000 | -120(110)  | 20(6)  | 2           | 19 min           |
| 23 Nov 2023 | 4983.000 | -116(110)  | 12(5)  | 8           | 94 min           |

TABLE IV  
INRIM-POLITO FDIB MEASUREMENT RESULTS FOR THE  $C_2:R_1$  RATIO AT 1541.434 Hz  
COMPARED WITH THE METAS DJIB RESULTS

| Date        | $\frac{(C_2^{\text{INRIM}} - C_2^{\text{METAS}})/C_2^{\text{nom}}}{\text{nF/F}}$ | $\frac{G_2^{\text{INRIM}} - G_2^{\text{METAS}}}{\text{nS}}$ | Repetitions | Measurement time |
|-------------|--|---|-------------|------------------|
| 09 Nov 2023 | -2(78)   | -0.958(31)  | 2           | 30 min           |
| 09 Nov 2023 | -304(78)   | -0.956(31)  | 6           | 77 min           |
| 04 Dec 2023 | -27(81)  | -0.562(80)  | 8           | 74 min           |

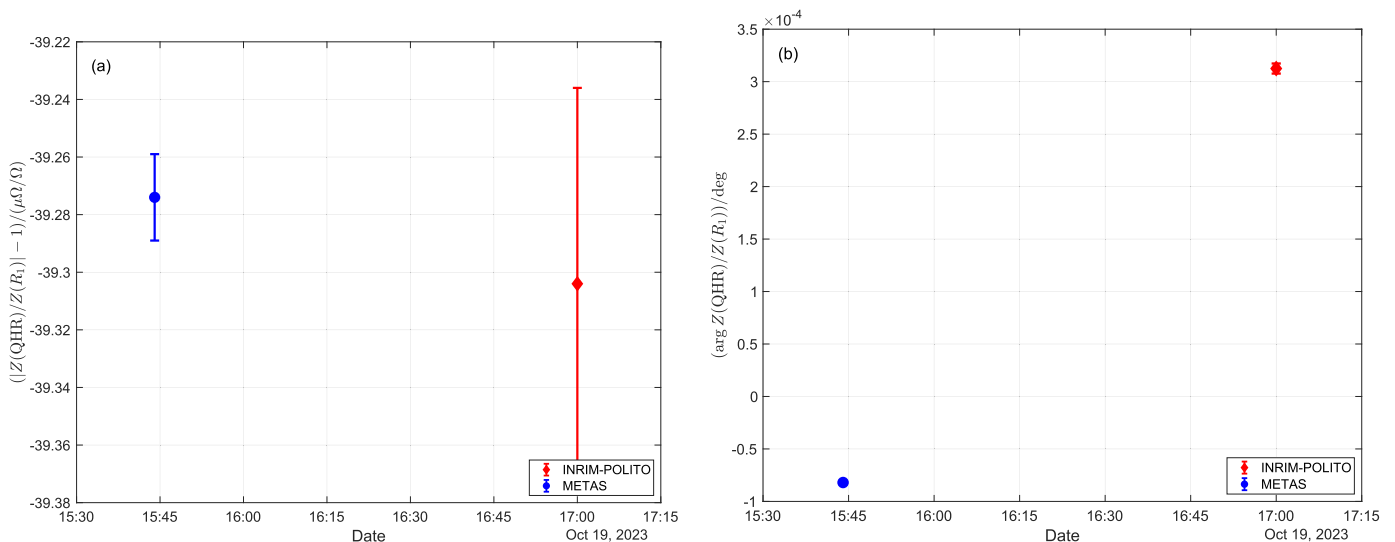


Fig. 6. Measurement results for the  $R_{\text{QHR}}:R_1$  ratio at 1233.147 Hz. (a) Deviation from the unit of the impedance magnitude ratio,  $|Z(R_{\text{QHR}})/Z(R_1)|$ . (b) Angle of the impedance ratio,  $\arg Z(R_{\text{QHR}})/Z(R_1)$ . The uncertainty bars represent the standard uncertainties with coverage factor  $k = 1$ .

dashed line in plot (a) represents the least-squares fit of the METAS DJIB measurements, indicating a relative drift coefficient  $(dC_1/dt)/C_1 \approx 13 \times 10^{-9} \text{ d}^{-1}$ . Since  $C_1$  is of recent construction, this result yielded a preliminary characterization of its stability. The drift of  $R_1$  was measured in dc during the same period being  $(dR_1/dt)/R_1 \approx 2 \times 10^{-9} \text{ d}^{-1}$ .

The plots in Fig. 5(a) and (b) show the results for the  $R_2:R_1$  ratio measurements at 1233.147 Hz. As in the previous case, the magnitude ratio results are compatible with the expanded uncertainties with coverage factor  $k = 2$ , and the phase measurements for the INRIM-POLITO FDIB deviate significantly from the other measurements before October 29. After this date, there is full compatibility also on the phase measurements. Indeed, the bridge network set for  $R:R$  ratio measurement is intrinsically more symmetric under impedance reversal with respect to the case of  $R:C$  ratio measurements, and the problem of uncompensated asymmetries is here less significant. The plots in Fig. 5(c) and (d) show the results for

the  $R_2:R_1$  ratio measurements at 5000 Hz. These measurements were performed before October 29, and the reported INRIM-POLITO FDIB result at 5000 Hz is incompatible with the other two results. Both the magnitude and phase discrepancies were removed after October 29 by the full exchange of the impedances (see the results in the Appendix).

## V. CONCLUSION

Onsite comparisons have always been an invaluable tool to validate and improve measuring systems at the highest level of accuracy because, with rare exceptions (see [23]), traveling standards do not typically have enough stability. Moreover, onsite comparisons allow NMIs to access a wide range of standards in the same place at the same time. The results herewith presented confirm the significance of onsite comparisons and the diagnostic power that these have in highlighting issues that could go undetected otherwise.

This comparison and the previous one reported in [5] both performed within the framework of the project EURAMET TC-EM 1501, *technical assessment of novel digital impedance bridges*, have demonstrated that dual Josephson impedance bridges and electronic fully digital impedance bridges perform with state-of-the-art accuracy in the kilohertz frequency range, and these kind of bridges allow NMIs to realize the unit of capacitance directly from a calculable resistance standard or, with some more technical care, from the quantum Hall effect.

It should be finally noted that impedance comparisons are typically limited to the primary parameters of the compared impedances (resistance, capacitance, or inductance), and the secondary parameters (time constant, dissipation factor, or series resistance), which are related to the impedance phase angle, are not considered quantities of interest. This comparison has instead shown that phase angle measurements need to be considered for complete characterization and perfection of impedance measuring systems (see also [3]).

#### APPENDIX FURTHER RESULTS

This section reports measurements from the INRIM-POLITO and METAS bridges only, and we have chosen to display the results mostly in the form of tables because each impedance pair was measured for at most a day or two.

Table III reports the results for the  $R_2:R_1$  ratio measurements at around 1 and 5 kHz with the INRIM-POLITO FDIB only. For this measurement, the two calculable resistance standards  $R_1$  and  $R_2$  were calibrated against the dc QHR standard by means of a cryogenic current comparator (CCC), and then, the ac/dc transfer coefficients were used to calculate the reference resistance values  $R_1^{\text{REF}}$  and  $R_2^{\text{REF}}$ , and the reference time constant values  $\tau_1^{\text{REF}}$  and  $\tau_2^{\text{REF}}$  at the frequencies of interest. The ratio  $Z(R_2)/Z(R_1)$  was measured with the INRIM-POLITO FDIB, and values  $R_2$  and  $\tau_2$  were determined from  $R_1^{\text{REF}}$  and  $\tau_1^{\text{REF}}$ . Table III reports the deviations of the measured values  $R_2$  and  $\tau_2$  from the reference values  $R_2^{\text{REF}}$  and  $\tau_2^{\text{REF}}$ . The reported uncertainties are only those due to the INRIM-POLITO FDIB, not considering the uncertainties of  $R_1^{\text{REF}}$ ,  $R_2^{\text{REF}}$ ,  $\tau_1^{\text{REF}}$ , and  $\tau_2^{\text{REF}}$ . Taking into account that the uncertainty of  $\tau_2^{\text{REF}}$  is about 100 ps, all measurements are compatible in both magnitude and phase. At 1 kHz, the measurement time for one repetition is about 8 min, whereas, at 5 kHz, the measurement time for one repetition increases at about 12 min. This is due to the fact that the waveforms at 5 kHz are synthesized with fewer samples, thus reducing the adjustment resolution.

Table IV reports the results for the  $C_2:R_1$  ratio measurements at 1541.434 Hz performed with both the INRIM-POLITO FDIB and the METAS DJIB. The number of repetitions and the measurement time are those of the INRIM-POLITO FDIB. For this measurement, the calculable resistance standard  $R_1$  was calibrated against the dc QHR standard by means of the CCC, and then, the ac/dc transfer coefficients were used to calculate the reference resistance value  $R_1^{\text{REF}}$  and the reference time constant value  $\tau_1^{\text{REF}}$  at the frequency of interest. The ratio  $Z(C_2)/Z(R_1)$  was measured

with both the INRIM-POLITO FDIB and the METAS DJIB, and values  $C_2^{\text{INRIM}}$ ,  $G_2^{\text{INRIM}}$ ,  $C_2^{\text{METAS}}$ , and  $G_2^{\text{METAS}}$  were determined from  $R_1^{\text{REF}}$  and  $\tau_1^{\text{REF}}$ .

The November 9 measurement with the INRIM-POLITO FDIB consisted of eight successive repetitions, which have been split into two parts in Table IV. For the first two repetitions, the results for  $C_2$  are well compatible, but, for the next six repetitions, the results are clearly no longer compatible. This phenomenon was likely due to the fact that  $C_2$  was first connected to the METAS DJIB with the shorter cables (about 2 m long) and then to the INRIM-POLITO FDIB with the longer cables (about 4 m long), and this caused a thermal transient in the capacitance standard due to the change in the thermal load toward the ambient. This thermal transient then caused a change in the capacitance during the measurement. This problem was solved during the December 4 measurement, in which the 4-m-long cables were used with both bridges and the capacitance value remained stable.

Table IV also shows that the measurement results for  $G_2$  are not compatible. This is again due to the incompatibility of phase measurements discussed in Section IV.

Finally, the plots in Fig. 6 show the results for the  $R_{\text{QHR}}:R_1$  ratio measurements performed at 1233.147 Hz with both the INRIM-POLITO FDIB and the METAS DJIB. It should be noted that these measurements were taken on October 19, before the full exchange of the impedances in the INRIM-POLITO FDIB, and the results are similar to those of Fig. 5 on the same date at the same frequency: the magnitude ratio results are compatible, whereas the phase results are incompatible. The phase deviation between the INRIM-POLITO FDIB and the METAS DJIB measurements is the same in Figs. 5 and 6 (there is a fictitious change of sign, which is just due to the connection order of the impedances). Later measurements with the QHR standard revealed a malfunction of the INRIM-POLITO FDIB when connected to the QHR network due to an interaction with the active current equalizers employed at METAS. This interaction was likely caused by an unwanted ground loop current that shifted the balance of the bridge, which unfortunately could not be eliminated during the time of the comparison. For this reason, the result with the INRIM-POLITO FDIB from Fig. 6 should be considered with caution.

#### REFERENCES

- [1] F. Overney and B. Jeanneret, "Impedance bridges: From wheatstone to Josephson," *Metrologia*, vol. 55, no. 5, pp. S119–S134, Oct. 2018.
- [2] G. Trenkler, "Digitalmeßbrücke zum vergleich von wirk- und blindwiderständen," *tm Technisches Messen*, vol. 503, no. 1, pp. 313–314, 1978.
- [3] M. Ortolano et al., "An international comparison of phase angle standards between the novel impedance bridges of CMI, INRIM and METAS," *Metrologia*, vol. 55, no. 4, pp. 499–512, Aug. 2018.
- [4] M. Marzano, *Technical Assessment of Novel Digital Impedance Bridges*. Accessed: Feb. 20, 2025. [Online]. Available: <https://www.euramet.org/technical-committees/tc-projects/details/project/technical-assessment-of-novel-digital-impedance-bridges>
- [5] M. Marzano et al., "PTB–INRIM comparison of novel digital impedance bridges with graphene impedance quantum standards," *Metrologia*, vol. 59, no. 6, Dec. 2022, Art. no. 065001.
- [6] M. Marzano et al., "Trilateral comparison among digital and Josephson impedance bridges," in *Proc. Conf. Precis. Electromagn. Meas. (CPEM)*, Jul. 2024, pp. 1–2.



- [7] R. D. Cutkosky, "Four-terminal-pair networks as precision admittance and impedance standards," *IEEE Trans. Commun. Electron.*, vol. CE-83, no. 70, pp. 19–22, Jan. 1964.
- [8] M. Ortolano et al., "A comprehensive analysis of error sources in electronic fully digital impedance bridges," *IEEE Trans. Instrum. Meas.*, vol. 70, 2021, Art. no. 1500914.
- [9] F. Overney et al., "Longitudinal impedance measurements on graphene QHE devices," in *Proc. Conf. Precis. Electromagn. Meas. (CPEM)*, Denver, CO, USA, Jul. 2024, pp. 1–2.
- [10] K. Musioł, M. Koszarny, M. Kampik, K. Kubiczek, A. Ziótek, and J. Jursza, "A new impedance metrology infrastructure at GUM," in *Proc. 25th IMEKO TC4 Int. Symp. 23rd Int. Workshop ADC DAC Model. Test.*, vol. 21. Budapest, Hungary: IMEKO, 2022, pp. 243–247.
- [11] J. Kucera and J. Kováč, "A reconfigurable four terminal-pair digitally assisted and fully digital impedance ratio bridge," *IEEE Trans. Instrum. Meas.*, vol. 67, no. 5, pp. 1199–1206, May 2018.
- [12] J. Kucera, J. Kováč, L. Palafox, R. Behr, and L. Vojáčková, "Characterization of a precision modular sinewave generator," *Meas. Sci. Technol.*, vol. 31, no. 6, Jun. 2020, Art. no. 064002.
- [13] J. Kováč and J. Kucera, "A modular coaxial multiplexer with high isolation between channels," in *Proc. 21st IMEKO World Congr.*, 2015, pp. 596–600.
- [14] J. Kaczmarek et al., "Virtual training laboratory for primary impedance metrology," *IEEE Trans. Instrum. Meas.*, vol. 72, pp. 1–12, 2023.
- [15] M. Marzano, M. Ortolano, V. D'Elia, A. Müller, and L. Callegaro, "A fully digital bridge towards the realization of the Farad from the quantum Hall effect," *Metrologia*, vol. 58, no. 1, Feb. 2021, Art. no. 015002.
- [16] A. Rüfenacht, N. E. Flowers-Jacobs, and S. P. Benz, "Impact of the latest generation of Josephson voltage standards in AC and DC electric metrology," *Metrologia*, vol. 55, no. 5, pp. S152–S173, Oct. 2018.
- [17] S. P. Benz and S. B. Waltman, "Pulse-bias electronics and techniques for a Josephson arbitrary waveform synthesizer," *IEEE Trans. Appl. Supercond.*, vol. 24, no. 6, pp. 1–7, Dec. 2014.
- [18] F. Overney, F. Lüönd, and B. Jeanneret, "Broadband fully automated digitally assisted coaxial bridge for high accuracy impedance ratio measurements," *Metrologia*, vol. 53, no. 3, pp. 918–926, Jun. 2016.
- [19] F. Overney et al., "Dual Josephson impedance bridge: Towards a universal bridge for impedance metrology," *Metrologia*, vol. 57, no. 6, Dec. 2020, Art. no. 065014.
- [20] F. Overney et al., "Josephson-based full digital bridge for high-accuracy impedance comparisons," *Metrologia*, vol. 53, no. 4, pp. 1045–1053, Jun. 2016.
- [21] S. Awan, B. Kibble, and J. Schurr, *Coaxial Electrical Circuits for Interference-Free Measurements* (Electrical Measurement Series). London, U.K.: Institution of Engineering and Technology, 2011.
- [22] J. Kucera, J. Kovac, and L. Bartova, "On alternative traceability chains of impedance units with digital impedance bridges," in *Proc. Conf. Precis. Electromagn. Meas. (CPEM)*, Jul. 2024, pp. 1–2.
- [23] S. Bauer, M. Götz, M. Kruskopf, and J. Schurr, "Long-term study on travelling standards for capacitance and resistance," in *Proc. Conf. Precis. Electromagn. Meas. (CPEM)*, Jul. 2024, pp. 1–2.



**Massimo Ortolano** was born in 1969. He received the M.Sc. degree in electronic engineering and the Ph.D. degree in metrology from the Politecnico di Torino, Turin, Italy, in 1997 and 2001, respectively.

Since 2000, he has been with the Department of Electronics and Telecommunications, Politecnico di Torino, where he is currently an Associate Professor. He teaches classes about electronic measurements and sensors. Since 2006, he has been collaborating with the Istituto Nazionale di Ricerca Metrologica (INRIM), Turin, with a focus on noise metrology,

modeling of quantum Hall effect devices, and impedance metrology. His research interests also include low current measurements, fundamental constants, time and frequency metrology, and statistical methods for the evaluation of uncertainty.



**Martina Marzano** was born in 1989. She received the M.Sc. degree in physics from the Università di Turin, Turin, Italy, in 2016, and the Ph.D. degree in metrology from the Politecnico di Torino, Turin, in collaboration with INRIM, Turin, in 2020, with a focus on novel devices and methods for quantum resistance and impedance metrology.

From 2018 to 2019 for six months at the National Institute of Standards and Technology, Gaithersburg, MD, USA. In 2021, she was a Guest Researcher for three months at PTB, Brunswick, Germany.

She is a Researcher with the Quantum Metrology and Nano Technologies Division at the Istituto Nazionale di Ricerca Metrologica/National Institute of Metrological Research (INRIM), Turin, Italy, from 2022, after a period as Post-Doctoral in the same division. Her current research at INRIM is focused on the development of new measurement methods and devices for resistance and impedance metrology.



**Frédéric Overney** (Member, IEEE) was born in Yverdon, Switzerland, on August 14, 1967. He received the M.S. degree in physics from the Swiss Federal Institute of Technology, Lausanne, Switzerland, in 1995.

He then joined with the Federal Institute of Metrology (METAS), Bern-Wabern, Switzerland, where he extended the measurement capabilities in the field of ac/dc transfer up to 1000 V and participated in the evaluation, modification, and characterization of an atomic clock comparison system based on GPS

signals. He has also been involved in the development of transformer-based coaxial ac bridges for studying the ac quantum Hall effect. His current work focuses on developing new measuring systems for impedance metrology, such as sampling bridges, digitally assisted bridges, and dual Josephson impedance bridges. In addition, he is working on designing new impedance standards with calculable frequency dependence over a broad frequency range, bridging the low-frequency to radio frequency (LF-RF) gap.



**Ali L. Eichenberger** received the Ph.D. degree in condensed matter physics, studying disordered 2-D Josephson junction arrays from the University of Neuchatel, Switzerland, in 1997.

He is a Physicist from the University of Neuchatel. From 1997 to 2000, he was a Guest Researcher at NIST, Boulder, CO, USA, where he participated in the development of a capacitance standard based on electron counting. In 2000, he joined the Swiss Federal Institute of Metrology METAS as a project leader of the Kibble balance experiment. Since 2023,

he has been responsible for the cryogenics laboratory, in particular for DC voltage and resistance measurements.



**Jan Kucera** was born in 1980. He received the M.Sc. degree in measurement and instrumentation and the Ph.D. degree in measurement techniques from the Department of Measurements, Faculty of Electrical Engineering, Czech Technical University in Prague (CTU), Prague, Czech Republic, in 2005 and 2012, respectively.

Since 2007, he has been an Assistant Professor at the Department of Measurements, FEE, CTU, in Prague. From 2008 to 2011, he was involved in research on quantum impedance metrology

with Physikalisch-Technische Bundesanstalt, Brunswick, Germany. In 2011, he joined Czech Metrology Institute, Prague, where he is engaged in primary metrology of dc resistance and electrical impedance quantities.



**Vincenzo D'Elia** was born in 1965. He received the High School degree in electronics from the Technical School G. Plana, Turin, Italy, in 1988.

He was with a telecommunication company. In 1996, he joined the Istituto Nazionale di Ricerca Metrologica, Turin, INRIM (formerly Istituto Elettrotecnico Nazionale Galileo Ferraris, IEN), where he is currently a Senior Technician. His current research interests include impedance metrology, ac voltage ratio, and low dc measurements.



**Juan Medved** (Graduate Student Member, IEEE) was born in 1997. He received the master's degree in electronics engineering from the Universidad Tecnológica Nacional (UTN-FRBA), Buenos Aires, Argentina, in 2022. He is currently pursuing the Ph.D. degree in electrical, electronics, and communications engineering at Politecnico di Torino, Turin, Italy, with a focus on quantum electrical impedance metrology.

He worked at the Quantum Metrology Group of the Instituto Nacional de Tecnología Industrial (INTI), Buenos Aires, and since 2023, he has been working with the Quantum Electronics and Nano Technologies Department at the Istituto Nazionale di Ricerca Metrologica (INRIM), Turin. His research interests include quantum Hall devices, Josephson standards, and impedance metrology.



**Luca Callegaro** (Member, IEEE) was born in 1967. He received the M.Sc. degree in electronic engineering and the Ph.D. degree in physics from Politecnico di Milano, Milano, Italy, in 1992 and 1996, respectively.

He is with the Istituto Nazionale di Ricerca Metrologica (INRIM), Turin, Italy, since 1996, where he currently serves as head of the Quantum Electronics Section. He has authored about 120 articles in international reviews and the book *Electrical Impedance: Principles, Measurement and Applications*, 2012.

He is responsible for the Italian National standards of electrical capacitance, inductance, ac resistance, and ac voltage ratio.

Dr. Callegaro is the Italian deputy delegate to EURAMET, the European Association of National Metrology Institutes, and the contact person of its Technical Committee for Electricity and Magnetism (TC-EM), in which he served four years as Chairperson. He is the Italian delegate to the Consultative Committee for Electricity and Magnetism (CCEM) of the International Committee for Weights and Measures (CIPM) and Vice-Chair of the Technical Committee TC4–Measurement of Electrical Quantities–of the International Measurement Confederation (IMEKO).

**Lucie Bartova**, photograph and biography not available at the time of publication.