

Mid-term Performance and Calibration of Multi-sensor Low-Cost Systems for Air Quality Monitoring in Urban Environments

*Original*

Mid-term Performance and Calibration of Multi-sensor Low-Cost Systems for Air Quality Monitoring in Urban Environments / Fellini, S., Gallione, D., Vaccaro, V., Mastromatteo, N., Fattoruso, G., Clerico, M., Salizzoni, P.. - In: AEROSOL AND AIR QUALITY RESEARCH. - ISSN 1680-8584. - ELETTRONICO. - (2026), pp. 1-37. [10.1007/s44408-026-00150-1]

*Availability:*

This version is available at: 11583/3013519 since: 2026-07-24T12:48:07Z

*Publisher:*

Springer Nature

*Published*

DOI:10.1007/s44408-026-00150-1

*Terms of use:*

This article is made available under terms and conditions as specified in the corresponding bibliographic description in the repository

*Publisher copyright*

Springer postprint/Author's Accepted Manuscript

This version of the article has been accepted for publication, after peer review (when applicable) and is subject to Springer Nature's AM terms of use, but is not the Version of Record and does not reflect post-acceptance improvements, or any corrections. The Version of Record is available online at: <http://dx.doi.org/10.1007/s44408-026-00150-1>

(Article begins on next page)

# Mid-term Performance and Calibration of Multi-sensor Low-Cost Systems for Air Quality Monitoring in Urban Environments

Received: 21 July 2025

Accepted: 23 June 2026

Published online: 03 July 2026

Cite this article as: Fellini S., Gallione D., Vaccaro V. *et al.* Mid-term Performance and Calibration of Multi-sensor Low-Cost Systems for Air Quality Monitoring in Urban Environments. *Aerosol Air Qual. Res.* (2026). <https://doi.org/10.1007/s44408-026-00150-1>

Sofia Fellini, Davide Gallione, Vincenzo Vaccaro, Nicole Mastromatteo, Grazia Fattoruso, Marina Clerico & Pietro Salizzoni

We are providing an unedited version of this manuscript to give early access to its findings. Before final publication, the manuscript will undergo further editing. Please note there may be errors present which affect the content, and all legal disclaimers apply.

If this paper is publishing under a Transparent Peer Review model then Peer Review reports will publish with the final article.

# Mid-term performance and calibration of multi-sensor low-cost systems for air quality monitoring in urban environments

Sofia Fellini<sup>1\*†</sup>, Davide Gallione<sup>1†</sup>, Vincenzo Vaccaro<sup>1</sup>,  
Nicole Mastromatteo<sup>1</sup>, Grazia Fattoruso<sup>3</sup>, Marina Clerico<sup>1</sup>,  
Pietro Salizzoni<sup>1,2</sup>

<sup>1\*</sup>Department of Environmental, Land and Infrastructure Engineering,  
Politecnico di Torino, Corso Duca degli Abruzzi, Turin, 10129, Italy.

<sup>2</sup>Laboratoire de Mécanique des Fluides et d'Acoustique, UMR CNRS  
5509, Université de Lyon, Ecole Centrale de Lyon, INSA Lyon,  
Université Claude Bernard Lyon I, Ecully, 69134, France.

<sup>3</sup>TERIN-SSI-EDS-LAB, ENEA CR-Portici, Portici, 80055, Italy.

\*Corresponding author(s). E-mail(s): [sofia.fellini@polito.it](mailto:sofia.fellini@polito.it);

†These authors contributed equally to this work.

## Abstract

This study evaluates mid-term calibration strategies for MONICA, a compact low-cost multi-sensor device for urban air quality monitoring, in the context of the upcoming EU Air Quality Directive 2024/2881. A key objective is to optimize the trade-off between calibration duration and long-term monitoring performance, balancing statistical robustness with practical deployment constraints. This question is particularly relevant in mid-latitude regions, where seasonal variability may introduce biases if calibration and observation periods are misaligned. Over a three-and-a-half-month winter co-location with reference-grade instruments, we assessed three models—Multiple Linear Regression (MLR), Random Forest (RF), and Generalized Additive Models (GAM)—across three pollutants: PM<sub>2.5</sub>, PM<sub>10</sub>, and NO<sub>2</sub>. MLR emerged as the most stable model for temporal extrapolation, while RF and GAM, although accurate short-term, showed performance degradation outside the training range. A two-week calibration period was sufficient for PM, whereas NO<sub>2</sub> required only one week. Although sensor accuracy declines over time—especially for NO<sub>2</sub>—the MONICA system remains effective in tracking temporal trends and identifying regulatory exceedances. These

results support the development of efficient and scalable low-cost sensor networks, offering practical insights for planning reliable air quality monitoring campaigns.

**Keywords:** keyword1, Keyword2, Keyword3, Keyword4

## 1 Introduction

Air pollution is a leading environmental health risk, contributing to millions of premature deaths annually through respiratory and cardiovascular diseases [e.g., 1–4]. Urban areas are particularly vulnerable due to high emission densities and complex morphologies that limit pollutant dispersion [5, 6].

Among urban air pollutants, particulate matter (PM) and nitrogen dioxide (NO<sub>2</sub>) remain the most critical due to their documented health effects and widespread exceedance of regulatory thresholds [7–9]. PM<sub>2.5</sub> is of particular concern due to its ability to penetrate deep into the respiratory system [10, 11], while NO<sub>2</sub> is strongly associated with respiratory inflammation [12–14]. These pollutants are regulated under the updated European Directive 2024/2881 [15], which tightens air quality standards in line with WHO recommendations and the European Green Deal’s zero-pollution ambition.

Accurately estimating ground-level concentrations in urban areas is essential for assessing individual exposure. However, pollutants exhibit high spatiotemporal variability [16, 17] that traditional, sparse monitoring networks, managed by environmental agencies, cannot fully capture. Consequently, understanding local air quality often relies on modeling approaches, including deterministic [18–21] and statistical models [22–24], whose application is often constrained by the available input data and the required spatial resolution.

In recent years, however, the emergence of low-cost sensors (LCS) has enabled high-resolution air quality monitoring, particularly in complex and heterogeneous urban environments [25]. Characterized by their compactness, low energy requirements, and affordability [26], LCS are increasingly used to create large-scale real-time monitoring networks that integrate both indoor and outdoor air quality measurements [27]. LCS systems have been successfully used to monitor air quality in areas lacking official stations, demonstrating their potential to enhance exposure assessments across diverse environments [28–31].

Despite their advantages, low-cost sensors still face significant challenges related to accuracy, precision, and durability [32–36]. To address these, LCS are commonly co-located with reference instruments for a calibration period, during which intra-sensor consistency (repeatability over time) and inter-sensor consistency (agreement between sensors and references) are assessed [27]. Importantly, the selection of a suitable calibration model is a critical step, and its appropriateness depends on the specific pollutant being measured.

PM sensor calibration commonly employs multiple linear regression and machine learning techniques [27, 37, 38]. These models often incorporate environmental variables like temperature and humidity, which are known to significantly influence sensor

output [39–41]. Research includes long-term co-location campaigns using large sensor datasets [36, 42] and assessment of the impact of specific conditions such as particle sources or relative humidity on measurement performance [32, 35]. Reviews by Venkattraman Jagatha et al. [37] and Giordano et al. [36] have highlighted both the promise and variability in sensor behavior and calibration strategies.

For NO<sub>2</sub>, the literature is more limited and the calibration performances are generally less robust. Previous studies have employed multiple linear regression [43–45], while others have tested machine learning approaches, including random forests [46, 47] and neural networks [48]. These works underline the importance of both long-term calibration and the inclusion of environmental covariates to mitigate sensor drift and improve prediction accuracy.

Although previous studies have provided important insights, several key limitations remain. In particular, few works have systematically evaluated calibration strategies for integrated multi-sensor systems measuring both PM and gaseous pollutants simultaneously [43, 49–51]. This is a significant gap, given the increasing use of such platforms in urban air quality networks. Moreover, calibration duration is seldom systematically assessed, despite its crucial role in ensuring model reliability under the temporal constraints typical of open-field monitoring deployments. There is currently no standardized co-location duration, and the reported co-location durations in recent works have varied from several days to several months [52]. This issue is especially relevant for non-linear and data-driven models which may suffer from reduced generalizability when applied beyond the temporal range of their training data [46]. The long-term stability of calibrated sensors and the performance decay also remain poorly understood. These uncertainties hinder the effective deployment of LCS, especially in long-term monitoring where recalibration is costly or logistically challenging.

To address these limitations, this study evaluates the MONICA device [53–57]. This integrated platform allows for multi-pollutant monitoring, relevant for urban-scale networks. We assess three calibration models (Multiple Linear Regression, MLR; Random Forest, RF; and Generalized Additive Models, GAM) across NO<sub>2</sub>, PM<sub>2.5</sub>, and PM<sub>10</sub>. The analysis addresses three core questions: (1) which calibration models provide the highest accuracy for each pollutant; (2) what is the minimum co-location period required to achieve stable and reliable calibration, depending on the model; and (3) for how long calibrated sensors maintain acceptable performance over time. A key focus of the study is to determine the maximum practical ratio between the calibration phase (2) and the total observation period (3). This is especially relevant for two reasons. First, in mid-latitude regions, extending the calibration period over several weeks or months may introduce seasonal biases if environmental conditions differ between the training and deployment phases. Second, given the limited lifespan of LCS (typically 1–2 years), an excessively long co-location phase limits the device’s actual monitoring utility.

The campaign was conducted in the city of Turin (Po Valley), one of Europe’s major air pollution hotspots, where persistent pollution levels are driven by intense local emissions and unfavorable meteorological conditions [58].

This work offers operational guidance for LCS-based campaigns, optimizing calibration strategies for robust and scalable monitoring networks for urban air pollution assessment.

## 2 Material and Methods

The experimental campaign was conducted in Turin, Italy, over a period of approximately four months, from November 6, 2023, to February 25, 2024. During this time, the MONICA multi-sensor systems were co-located with certified reference instruments at the DIATI (Department of Environment, Land and Infrastructure Engineering, Politecnico di Torino) monitoring station. This period allowed the systems to be exposed to a wide range of typical urban winter concentrations: hourly averaged concentrations of  $\text{NO}_2$  ranged from 3 to  $85 \mu\text{g}/\text{m}^3$ , while  $\text{PM}_{10}$  and  $\text{PM}_{2.5}$  varied between  $2\text{--}132 \mu\text{g}/\text{m}^3$  and  $1\text{--}132 \mu\text{g}/\text{m}^3$ , respectively. These data provided the basis for both the development (training) of the regression models and the subsequent validation of their temporal stability, as the sensors remained in the same location throughout the entire campaign.

### 2.1 MONICA low cost sensors

The ENEA MONICA device is a compact, cost-effective microsensor designed for air quality monitoring in both fixed and mobile applications. It is housed in a robust, waterproof enclosure (see box in Figure 1) with mesh-protected inlets to allow air exchange while preventing contamination from insects or debris. Inside the box, the monitoring setup includes both the MONICA sensor and a Raspberry Pi unit. The Raspberry Pi communicates with the MONICA device via Bluetooth to receive raw data, and—when connected to the local Wi-Fi network—it transfers the collected data to a cloud-based storage and visualization platform. The Raspberry Pi also allows for local access to raw files and remote control via RealVNC, enabling troubleshooting and system monitoring when necessary.

The MONICA system incorporates a Plantower PMS7003 optical particle counter [59] and several electrochemical sensors for gas monitoring: the Alphasense CO-A4 [60] for carbon monoxide, the NO2-A43F [61] for nitrogen dioxide, and the OX-A431 [62] for ozone detection. The MONICA device also records meteorological parameters such as temperature (T) and relative humidity (rH) via a DHT22 sensor [63]. Details regarding the measurement ranges for the sensors deployed in this study are summarized in Table 1.

The MONICA system estimates  $\text{NO}_2$  concentrations using the voltage signals from two electrochemical sensors: the  $\text{NO}_2$ -selective sensor (NO2-A43F) and the OX-A431 sensor, which is primarily sensitive to ozone but also exhibits cross-sensitivity to  $\text{NO}_2$ . Both sensors (Alphasense A4 series) provide outputs from a working electrode (WE) and an auxiliary electrode (AE); the latter is specifically designed to physically compensate for temperature-dependent baseline shifts [64, 65]. The corresponding signals ( $\text{NO}_2\text{WE}$ ,  $\text{NO}_2\text{AE}$ ,  $\text{NO}_2\text{O}_3\text{WE}$ ,  $\text{NO}_2\text{O}_3\text{AE}$ ) are used to correct the  $\text{NO}_2$  response by accounting for both thermal drift and ozone interference [64, 65].

Particulate matter concentrations are derived from the optical particle counter. It provides mass concentrations under standard conditions ( $\text{PM}_{2.5\text{SP}}$ ,  $\text{PM}_{10\text{SP}}$  in Table 1), assuming a reference particle size distribution and dry aerosol state. Since field conditions rarely conform to these assumptions, the system also provides adjusted values ( $\text{PM}_{2.5\text{AE}}$ ,  $\text{PM}_{10\text{AE}}$  in Table 1) that account for ambient temperature and


relative humidity. These corrections are applied using a factory-defined regression model, which internally adjusts the raw signals based on typical atmospheric responses. However, this model is not site-specific: the regression parameters are predefined by the manufacturer and remain fixed across locations and conditions.

Additionally, the MONICA device reports particle number concentrations for particles larger than  $2.5 \mu\text{m}$  ( $\text{NP}_{2.5}$ ) and  $10 \mu\text{m}$  ( $\text{NP}_{10}$ ), which provide complementary information on aerosol number and size distribution.

Data collected by MONICA are transmitted in real-time to a dedicated web platform, where users can visualize measurements through time-series graphs and location-based air quality maps.

**Table 1** Sensor output parameters from the ENEA MONICA low-cost system relevant to the measurement of  $\text{NO}_2$ ,  $\text{PM}_{2.5}$ ,  $\text{PM}_{10}$ , temperature and humidity. Sensor models and their manufacturer-specified measurement ranges are provided in the final column.

| Nitrogen dioxide – $\text{NO}_2$ |                                                                                                   |                                                            |
|----------------------------------|---------------------------------------------------------------------------------------------------|------------------------------------------------------------|
| $\text{NO}_2\text{WE}$           | Terminal voltage (mV) - Working Electrode, sensitive primarily to $\text{NO}_2$                   | Alphasense $\text{NO}_2\text{-A43F}$<br>Range: 0-20 ppm    |
| $\text{NO}_2\text{AE}$           | Terminal voltage (mV) - Auxiliary Electrode, for interference compensation                        |                                                            |
| $\text{NO}_2\text{O}_3\text{WE}$ | Terminal voltage (mV) - Working Electrode, sensitive to $\text{O}_3$ and $\text{NO}_2$            | Alphasense $\text{OX-A431}$                                |
| $\text{NO}_2\text{O}_3\text{AE}$ | Terminal voltage (mV) - Auxiliary Electrode, for interference compensation                        | Range: 0-20 ppm                                            |
| Particulate Matter – PM          |                                                                                                   |                                                            |
| $\text{PM}_{2.5}\text{SP}$       | $\text{PM}_{2.5}$ concentration ( $\mu\text{g}/\text{m}^3$ ) - under standard particle conditions | Plantower PMS7003 Range:<br>0-500 $\mu\text{g}/\text{m}^3$ |
| $\text{PM}_{10}\text{SP}$        | $\text{PM}_{10}$ concentration ( $\mu\text{g}/\text{m}^3$ ) - under standard particle conditions  |                                                            |
| $\text{PM}_{2.5}\text{AE}$       | $\text{PM}_{2.5}$ concentration ( $\mu\text{g}/\text{m}^3$ ) under atmospheric conditions         |                                                            |
| $\text{PM}_{10}\text{AE}$        | $\text{PM}_{10}$ concentration ( $\mu\text{g}/\text{m}^3$ ) under atmospheric conditions          |                                                            |
| $\text{NP}_{2.5}$                | Number of particles with diameter $>2.5 \mu\text{m}$                                              |                                                            |
| $\text{NP}_{10}$                 | Number of particles with diameter $>10 \mu\text{m}$                                               |                                                            |
| Meteorological Parameters        |                                                                                                   |                                                            |
| rH                               | Relative Humidity (%)                                                                             | DHT22. Range:<br>0–100% RH; [-40, +80] °C                  |
| T                                | Air Temperature (°C)                                                                              |                                                            |

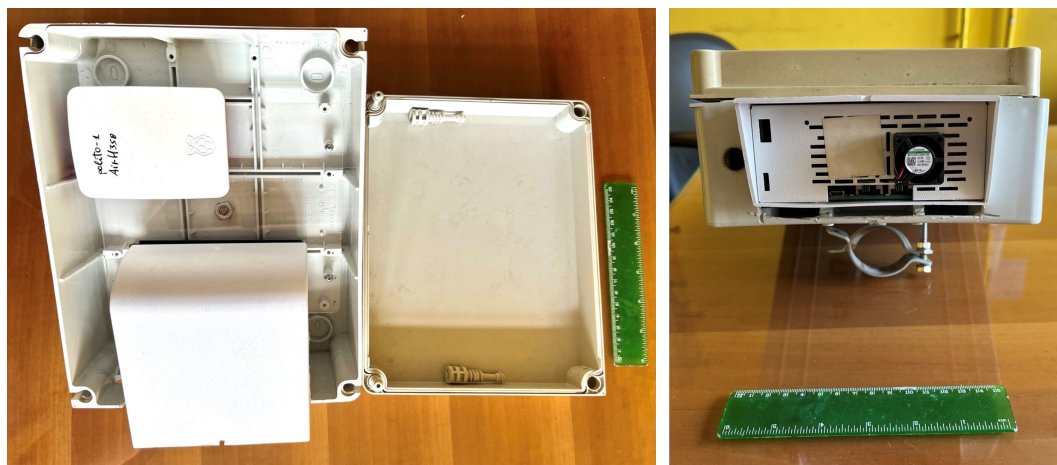

**Fig. 1** ENEA MONICA device. Left: Internal view of the device. Right: Close-up of the chamber housing the PM and NO<sub>2</sub> microsensors. The overall dimensions of the device are  $19 \times 24 \times 10 \text{ cm}^3$ , and the microsensor chamber measures  $12.5 \times 13.5 \times 6 \text{ cm}^3$ . A 15 cm ruler is placed next to the device for scale reference.

## 2.2 Certified instruments for sensor calibration and validation

Two air quality monitoring stations were used to provide reference measurements for the calibration and validation of the MONICA sensors: the fixed station CC-Green Roof Lab (Figure 2, left) and the mobile laboratory CC-TrAIRer Lab [66] (Figure 2, right). Both stations are equipped with certified instruments for air quality and meteorological monitoring.

Specifically, the following reference instruments were used in this study: a Palas Fidas 200S (2 in Figure 2) for particulate matter (PM<sub>2.5</sub> and PM<sub>10</sub>), an Envea AC32e analyzer (3 in Figure 2) and a Serinus 40 analyzer (4 in Figure 2) for NO<sub>2</sub>, and a Davis Vantage Pro 2 weather station (5 in Figure 2) for temperature, relative humidity, precipitation, wind speed, and direction.



**Fig. 2** Positioning of ENEA MONICA microsenors and reference instruments for calibration at DIATI – Politecnico di Torino. Left: CC-Green Roof. Right: CC-TrAIRer Lab. 1 – ENEA MONICA™ microsenors, 2 – Palas Fidas 200S optical sensor for PM measurement, 3 – Sampling head for ENVEA AC32e analyzer for NO<sub>2</sub> measurements, 4 – Sampling head for Serinus 40 analyzer for NO<sub>2</sub> measurements, 5 – Davis Vantage Pro 2 weather station.

The Palas Fidas 200S is an optical spectrometer designed for atmospheric pollution monitoring, certified according to the EN 16450 standard. It enables continuous and simultaneous measurement of various particulate fractions: PM<sub>1</sub>, PM<sub>2.5</sub>, PM<sub>4</sub>, PM<sub>10</sub>, and total suspended particles (TSP), along with particle number concentration and size distribution. The measurement range is 0.18  $\mu\text{m}$  to 18  $\mu\text{m}$ . For this study, only PM<sub>2.5</sub> and PM<sub>10</sub> data were used.

The Serinus 40 NO<sub>x</sub> Analyzer is a high-precision instrument designed to measure nitrogen oxides using the gas-phase chemiluminescence method. Ambient air, pre-filtered through 47 mm Teflon filters to remove large particles, enters the reaction cell through two alternating pathways dedicated to nitric oxide (NO) and nitrogen oxides (NO<sub>x</sub>) measurements. In the first pathway, atmospheric NO reacts with O<sub>3</sub>, producing a chemiluminescent signal proportional to its concentration. In the second pathway, the airflow passes through a delay loop and an NO<sub>2</sub>-to-NO converter. The delay loop, a coiled flow circuit, ensures proper separation of the two measurement sequences, enabling the sequential detection of NO and total NO<sub>x</sub>.

The ENVEA AC32e is an eco-designed reference air quality monitor that utilizes the chemiluminescence principle, which is the standard method for measuring NO<sub>2</sub> and NO concentrations in ambient air (certified according to EN 14211). To measure NO<sub>x</sub>, the instrument passes the sample through a heated catalyst, which converts all nitrogen oxides into NO. By alternately introducing and bypassing the catalyst in the sample path, the analyzer compares the resulting signals, allowing for the indirect quantification of NO<sub>2</sub>.

205 The Davis Vantage Pro 2 weather station is designed to monitor and record data  
 206 related to the weather and climate conditions of a location, with variable frequency.  
 207 The measured parameters include temperature, atmospheric pressure, humidity, wind  
 208 speed and direction, solar radiation, rainfall rate, and ultraviolet radiation.

### 209 2.3 Regression models for calibration of the LCS

210 Accurate calibration of the MONICA low-cost sensor system is essential to correct  
 211 for environmental interferences and sensor-specific variability [64, 65]. In this study,  
 212 the MONICA device was colocated with the DIATI reference stations described in  
 213 Section 2.2. During the co-location period, MONICA sensor outputs were paired with  
 214 hourly reference measurements of NO<sub>2</sub>, PM<sub>2.5</sub>, and PM<sub>10</sub>. These data were used  
 215 to train regression models capable of translating raw sensor signals (e.g., electrode  
 216 voltages and particle counts) into calibrated pollutant concentrations. This in-field  
 217 calibration addresses limitations of factory-set models, which do not adapt to local  
 218 environmental conditions [52, 67].

219 We applied three different regression models commonly used in the literature to  
 220 calibrate the MONICA devices.

221 The first model is a Multiple Linear Regression (MLR) [68] of the following form:

$$Y = \alpha_0 + \alpha_1 X_1 + \alpha_2 X_2 + \cdots + \alpha_n X_n, \quad (1)$$

222 where  $Y$  is the predicted target variable,  $\alpha_0$  is the intercept,  $\alpha_1, \alpha_2, \dots, \alpha_n$  are the  
 223 coefficients for each predictor, and  $X_1, X_2, \dots, X_n$  are the input features.

224 The second model is a Generalized Additive Model (GAM) with smoothing splines  
 225 applied to each predictor [69]. GAMs extend linear models by allowing non-linear  
 226 relationships, providing a more flexible framework to capture subtle trends in the data.  
 227 The equation for a GAM can be represented as:

$$Y = f_1(X_1) + f_2(X_2) + \cdots + f_n(X_n), \quad (2)$$

228 where  $Y$  is the predicted target variable,  $f_1(X_1), f_2(X_2), \dots, f_n(X_n)$  are smoothing  
 229 functions of each predictor.

230 The third model is a Random Forest (RF) regressor. Random forests are ensemble  
 231 methods that combine multiple decision trees to improve predictive accuracy and  
 232 mitigate overfitting through averaging [70]. The general equation is:

$$Y = \frac{1}{n} \sum_{i=1}^n T_i(X), \quad (3)$$

233 where  $Y$  is the predicted target variable,  $n$  is the number of trees,  $T_i(X)$  is the output  
 234 of the  $i^{\text{th}}$  decision tree, and  $X$  is the input feature vector. This approach is particu-  
 235 larly effective for capturing non-linear dependencies and complex interactions between  
 236 variables. The RF model was implemented using the *scikit-learn* library in Python.  
 237 The number of trees (200) was selected based on a sensitivity analysis where the Root  
 238 Mean Square Error (RMSE) was evaluated as a function of the number of trees. We

observed that the model performance stabilized well before reaching 200 trees; therefore, this value was chosen as an optimal trade-off between predictive accuracy and computational efficiency. While increasing the number of trees typically does not, by itself, induce overfitting (as predictions are obtained through ensemble averaging [71]) it is recognized that beyond a certain complexity, adding further trees generally yields diminishing returns in performance while increasing the computational burden. Consequently, the chosen threshold was deemed sufficient to ensure both model stability and generalizability without unnecessary complexity. To ensure reproducibility, a fixed random seed (*random.state* = 42) was applied, while other hyperparameters were kept at their default settings to maintain a robust configuration for capturing non-linear relationships.

The calibration was performed using continuous time windows rather than shuffled data to prevent temporal data leakage and to evaluate the sensors' performance under realistic deployment conditions [46]. For the same reason, the "time of day" was not included as a predictor; avoiding site-specific temporal features reduces the risk of overfitting to local emission cycles and ensures better model transferability across different locations and periods.

For each pollutant, the regression models initially incorporated all meteorological parameters (temperature and relative humidity) along with pollutant-related parameters from the MONICA system (Table 1).

To optimize the model and ensure its robustness, a systematic feature selection was performed using an all-subset regression approach (implemented via the `best1m` R function). This procedure evaluated all possible combinations of predictors to identify the most effective subset for each pollutant. The selection process was based on maximizing the model's predictive accuracy while maintaining parsimony; specifically, parameters that did not provide a statistically significant improvement to the regression performance were subsequently excluded.

For illustrative purposes, the following multiple linear regression (MLR) equations correspond to the model calibrated using a two-week training period, which—as will be discussed in the following sections—represents a good trade-off between calibration effort and predictive performance:

$$\text{PM}_{2.5} = \alpha_0 + \alpha_1 \cdot \text{PM}_{2.5}\text{AE} + \alpha_2 \cdot \text{NP}_{2.5} + \alpha_3 \cdot \text{rH} \quad (4a)$$

$$\text{PM}_{10} = \beta_0 + \beta_1 \cdot \text{PM}_{10}\text{AE} + \beta_2 \cdot \text{PM}_{10}\text{SP} + \beta_3 \cdot \text{rH} \quad (4b)$$

$$\text{NO}_2 = \gamma_0 + \gamma_1 \cdot \text{NO}_2\text{WE} + \gamma_2 \cdot \text{NO}_2\text{O}_3\text{WE} + \gamma_3 \cdot \text{rH}. \quad (4c)$$

The regression coefficients from the two-week training period are reported in Table 2. These are dimensional coefficients, as the regression models were trained using the predictors in their original units without normalization.

The same predictor variables shown in Equations 4a-c were also used in the generalized additive model (GAM) and the random forest (RF) model.

As shown in Equations 4a-c, and in line with previous studies [57], relative humidity emerges as a key factor influencing sensor response. In contrast, no explicit dependence is observed between pollutant concentrations and temperature. This outcome,

**Table 2** Coefficients for MLR model (Equations 4) obtained from the two-week training period. The coefficients are dimensional and their magnitude reflects the specific scales of the raw sensor outputs (e.g., mV or particle counts).

| Pollutant         | Regression coefficients |                    |                     |                     |   |
|-------------------|-------------------------|--------------------|---------------------|---------------------|---|
| PM <sub>2.5</sub> | $\alpha_0 = 8.420$      | $\alpha_1 = 0.516$ | $\alpha_2 = -0.036$ | $\alpha_3 = -0.090$ |   |
| PM <sub>10</sub>  | $\beta_0 = 16.207$      | $\beta_1 = 0.541$  | $\beta_2 = -0.039$  | $\beta_3 = -0.152$  |   |
| NO <sub>2</sub>   | $\gamma_0 = -1328.265$  | $\gamma_1 = 4.468$ | $\gamma_2 = -0.137$ |                     | – |

resulting from the feature selection process, can be explained by the specific conditions of the winter campaign, where the observed temperature range was relatively narrow (0.6 to 20.9 °C), and a moderate Pearson correlation coefficient of 0.53 was found between  $T$  and rH. Under these specific conditions, the variance associated with temperature may be sufficiently captured by the humidity parameter, rendering  $T$  a redundant predictor for the algorithms. Furthermore, as detailed in Section 2.1, the MONICA sensors already incorporate hardware and firmware-level thermal compensations. Among the pollutant-related parameters, some were found to be more influential than others. For instance, the NP<sub>2.5</sub> parameter, which represents the number of PM<sub>2.5</sub> particles, was included in the regression model for PM<sub>2.5</sub> concentration. In contrast, the corresponding NP<sub>10</sub> parameter for PM<sub>10</sub> was excluded, as it did not contribute to improving the model’s accuracy.

As shown in Equation 4c and Table 2, the NO<sub>2</sub> model explicitly incorporates the NO<sub>2</sub>O<sub>3</sub>WE signal from the OX-A431 sensor to compensate for ozone interference. While O<sub>3</sub> levels were typically low during this winter campaign, including these terms ensures that the model is chemically consistent and remains robust against localized or transient fluctuations in ozone concentrations. Nevertheless, further testing during summer months would be necessary to fully assess the sensors’ performance under higher O<sub>3</sub> concentrations and broader temperature fluctuations, which could alter the weight of the ozone-correction term. In such scenarios, the inclusion of  $T$  might also become essential to maintain model stability.

## 2.4 Data processing and performance metrics

Although the monitoring campaign spanned the entire period from November 2023 to February 2024 (as described at the beginning of this section), several interruptions affected the operation of the reference instruments, reducing the time windows available for direct comparisons. Specifically, for PM<sub>2.5</sub> and PM<sub>10</sub>, comparisons were possible from 6 November 2023 to 5 January 2024, and again from 25 January to 25 February 2024. For NO<sub>2</sub>, valid comparison data were available from 6 November 2023 to 5 January 2024, and from 25 January to 4 February 2024.

For the training and evaluation periods, the analysis was organized by full weeks (Monday to Sunday), as field measurement campaigns are typically structured in this manner. As shown in Table A1 in the A, there were 12 full weeks available for particulate matter (PM<sub>2.5</sub> and PM<sub>10</sub>) and 9 full weeks for NO<sub>2</sub>. Only the weeks with complete data coverage are numbered.

To assess the agreement between measurements from the MONICA sensors and the reference instruments, we employed standard statistical indicators commonly recommended in the literature for evaluating correlation, error, and bias [9]. These include the coefficient of determination ( $R^2$ ), the Fractional Bias (FB), the Root Mean Square Error (RMSE), the Normalized Fractional Bias (NFB), and the Mean Geometric Bias (MGB). The selection of these metrics allows for a comprehensive evaluation of the sensor's accuracy, precision, and systematic errors, which are essential for low-cost sensor validation.

The definitions and mathematical expressions for these metrics are presented in Table 3, where the following symbols are used in the definitions:  $C_i$  denotes the concentration measured by the low-cost sensor for the  $i$ -th observation,  $C_{\text{ref},i}$  denotes the concentration measured by the reference instrument for the  $i$ -th observation,  $\bar{C}$  is the mean concentration provided by the low-cost sensor,  $\bar{C}_{\text{ref}}$  is the mean concentration provided by the reference instrument, and  $N$  represents the number of paired measurements.

$R^2$  quantifies the extent to which sensor measurements explain the variance in reference data and is widely used to evaluate correlation strength. Values above 0.7 indicate strong agreement, while values below 0.5 reflect weak predictive performance [72]. The Root Mean Square Error (RMSE) measures the average magnitude of error between sensor and reference measurements. As a key indicator of overall accuracy, lower RMSE values denote better agreement [73, 74]. In addition, the FB and NFB are commonly used indicators in sensor validation studies [e.g., 75, 76] to assess systematic errors between sensor and reference measurements. FB indicates relative bias, helping to detect consistent over- or underestimation, while NFB normalizes this measure, allowing for comparisons across sensors and varying concentration levels. Finally, we consider the geometric mean of the ratio between sensor and reference measurements (MGB). Unlike additive bias metrics, MGB is particularly valuable for capturing multiplicative errors, common in environmental measurements, where inaccuracies often scale with concentration levels. This is especially relevant when pollutant concentrations span multiple orders of magnitude, as traditional error metrics may disproportionately emphasize high-concentration deviations. By providing a scale-invariant measure of the bias, MGB ensures a more balanced evaluation across different concentration ranges [77].

### 3 Results

This section begins by describing the meteorological and air quality conditions observed during the measurement campaign (Section 3.1). It then evaluates the performance of different regression models applied to the MONICA system data (Section 3.2), followed by an analysis of the temporal stability of the calibration and the minimum duration required to achieve effective calibration (Section 3.3). Finally, it examines the capability of the low-cost sensors to detect exceedances of air quality thresholds defined by the new European Directive 2024/2881 (Section 3.4).

**Table 3** Mathematical definitions of the performance metrics used for sensor validation.

| Metric | Definition                                                                                      |
|--------|-------------------------------------------------------------------------------------------------|
| $R^2$  | $1 - \frac{\sum_{i=1}^N (C_i - C_{\text{ref},i})^2}{\sum_{i=1}^N (C_i - \bar{C})^2}$            |
| RMSE   | $\left[ \frac{1}{N} \sum_{i=1}^N (C_i - C_{\text{ref},i})^2 \right]^{0.5}$                      |
| FB     | $\frac{\sum_{i=1}^N (\bar{C}_i - \bar{C}_{\text{ref},i})}{\sum_{i=1}^N \bar{C}_{\text{ref},i}}$ |
| NFB    | $\frac{2 \sum_{i=1}^N (C_i - C_{\text{ref},i})}{\sum_{i=1}^N (C_i + C_{\text{ref},i})}$         |
| MGB    | $\exp \left( \frac{1}{N} \sum_{i=1}^N \ln \left( \frac{C_i}{C_{\text{ref},i}} \right) \right)$  |

### 3.1 Temporal analysis of meteorological data and pollutant concentration

Figure 3 illustrates the meteorological and air quality trends measured by the reference instruments (Section 2.2) during the monitoring period. For better visual clarity and to ensure a continuous time series, the figure focuses on the measurements collected from early November to late December 2023.


As is typical for the winter season in northern Italy, temperatures ranged from 0 to 15°C during the day, with occasional peaks nearing 20°C and an average temperature of approximately 8°C. The lowest temperatures were observed in the first week of December. Relative humidity ranged between 14% and 95%, maintaining above 60% in the first half of November and during the central part of December. Rainfall was almost absent.

Pollutant concentrations reveal significant temporal variability over the monitoring period, with particularly elevated levels of PM and NO<sub>2</sub> during the colder months. In early November, PM<sub>2.5</sub> reached daily maximum values around 30 µg/m<sup>3</sup>, and PM<sub>10</sub> peaked at approximately 50 µg/m<sup>3</sup>. In the second half of November, more pronounced fluctuations were observed, with daily concentrations reaching 50 µg/m<sup>3</sup> for PM<sub>2.5</sub> and 75 µg/m<sup>3</sup> for PM<sub>10</sub>. A further rise occurred in late December, where PM<sub>2.5</sub> remained consistently above 40 µg/m<sup>3</sup> and peaked at 80 µg/m<sup>3</sup>, while PM<sub>10</sub> exceeded 50 µg/m<sup>3</sup> on most days and reached values up to 100 µg/m<sup>3</sup>. However, considering the entire three-and-a-half-month campaign, pollution events were even more acute, with hourly peaks reaching 132 µg/m<sup>3</sup> for PM<sub>2.5</sub> and 132 µg/m<sup>3</sup> for PM<sub>10</sub>.

NO<sub>2</sub> concentrations followed a similar trend, gradually increasing through November and reaching hourly peaks of 50 µg/m<sup>3</sup>. In late December, NO<sub>2</sub> levels rose further, with hourly maximum values approaching 80 µg/m<sup>3</sup>. The absolute hourly maximum for the full campaign was recorded at 85 µg/m<sup>3</sup>.

The green dashed lines in the figure represent the daily mean limit values established by the new European Directive (EU) 2024/2881. During the monitoring period, the reference instruments frequently recorded concentrations above these thresholds, particularly for PM<sub>2.5</sub> and PM<sub>10</sub> in December. While these observations highlight the

critical air quality conditions of the site, a systematic analysis of the exceedances and the ability of the low-cost MONICA sensors to correctly identify them is provided in Section 3.4.

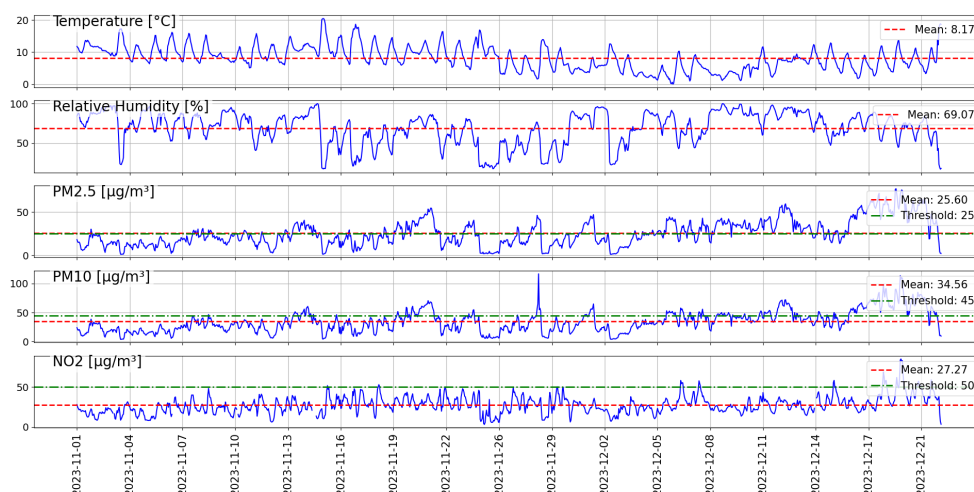

**Fig. 3** Hourly trend of meteorological parameters and pollutant concentrations measured by the fixed reference station of the Politecnico di Torino. From top to bottom: Temperature, Relative Humidity, PM<sub>2.5</sub>, PM<sub>10</sub>, and NO<sub>2</sub>. The green dashed lines in the figure represent the daily mean limit values established by the new European Directive (EU) 2024/2881.


## 3.2 Performance of the three regression models

The three regression models presented in Section 2.3 were trained using concentration data from the reference instruments and the predictor variables from the MONICA system listed in Table 1. While various training durations were tested (as discussed in the following sections), this subsection focuses on evaluating the performance of the three regression models during a standard two-week training phase, which serves as our baseline for comparison.

Figure 4 presents scatter plots comparing the hourly averaged concentrations derived from sensor measurements and those predicted by the regression models during the training phase. The RF model (third row) achieves the best overall performance, with  $R^2$  consistently above 0.95 across all pollutants. The GAM model performs slightly worse, particularly for NO<sub>2</sub>, with  $R^2$  dropping to 0.66 and higher RMSE values due to underestimation of peak concentrations. MLR shows a similar behavior but with slightly lower performance compared to the other models.

During the two-week training period, the concentration ranges measured were approximately 1-40  $\mu\text{g}/\text{m}^3$  for PM<sub>2.5</sub>, 4-60  $\mu\text{g}/\text{m}^3$  for PM<sub>10</sub>, 6-53  $\mu\text{g}/\text{m}^3$  for NO<sub>2</sub>. The regression models are thus trained on these concentration ranges.

The regression models calibrated on these two weeks, were then applied to the predictor values measured by the MONICA sensors in the following weeks. In Figure 5,

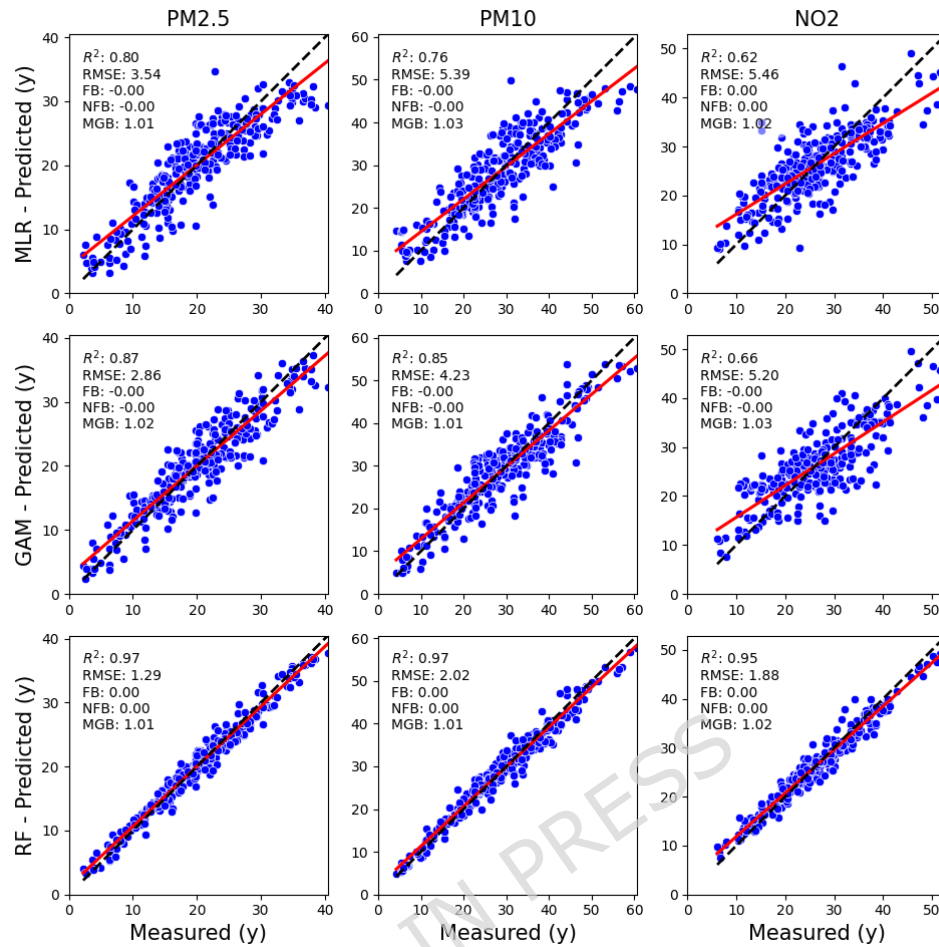

**Fig. 4** Scatter plots comparing the regression results of models trained over 2 weeks with the data measured during the same 2-week period. Each column corresponds to a pollutant (PM<sub>2.5</sub>, PM<sub>10</sub>, NO<sub>2</sub>), each row corresponds to a statistical indicator ( $R^2$ , FB, RMSE). Each point represents an hourly averaged concentration value, obtained by aggregating sensor measurements at hourly resolution.

the regression model results are compared to the reference instrument measurements during Week 7 (i.e., five weeks after the training period). The scatter plots in the first row show that the MLR regression model is able to accurately reconstruct pollutant concentrations, especially for particulate matter. For both PM<sub>2.5</sub> and PM<sub>10</sub>, data points align well with the bisector, and statistical indicators confirm a good agreement. However, NO<sub>2</sub> concentrations tend to be underestimated, as indicated by the negative values of the fractional bias.

In the second row, the scatter plots for the GAM model highlight a limitation in predicting high concentration values, especially for PM. At low and moderate concentrations, model performance is comparable to that of MLR, but at higher levels - beyond approximately  $40 \mu\text{g}/\text{m}^3$  for  $\text{PM}_{2.5}$  and  $50 \mu\text{g}/\text{m}^3$  for  $\text{PM}_{10}$  - the predicted values increasingly deviate from the bisector. This progressive divergence reduces the  $R^2$  and increases RMSE, indicating a deterioration in model performance. For  $\text{NO}_2$ , on the other hand, GAM predictions remain closer to the bisector across the concentration range and yield performance metrics similar to those of MLR.


The RF model (third row) exhibits a performance pattern comparable to the GAM but with a more pronounced *saturation* effect. While it accurately reproduces concentrations up to the training thresholds, it displays a characteristic flattening in the upper portion of the scatter plots. This behavior aligns with the inherent structural limitations of non-parametric models: unlike parametric approaches (e.g., MLR) that assume a global functional form, models like RF are strictly data-driven and cannot extrapolate beyond the training range [e.g., 46]. Specifically, predictions are constrained to the maximum values encountered during training because the ensemble cannot predict values outside the range of its leaf nodes.

The impact of this limitation varies depending on how far test values exceed the training range. For  $\text{PM}_{2.5}$  and  $\text{PM}_{10}$ , concentration levels during Week 7 reached levels nearly double the training maxima (up to  $80$  and  $110 \mu\text{g}/\text{m}^3$ , respectively). In this regime, the superior extrapolation capability of MLR clearly highlights the saturation effect of the RF model. Conversely, for  $\text{NO}_2$ , the performance gap is less pronounced. Although the RF model remains constrained by its training ceiling, the MLR benchmark itself exhibits significant underestimation at higher concentrations. Consequently, the inherent limitations of the non-parametric model are less evident for  $\text{NO}_2$ , as the linear reference also struggles to accurately capture the extreme values in that specific range.

These results emphasize the importance of including sufficient variability, particularly higher concentration episodes, in the training dataset when calibrating low-cost sensors with non-linear data-driven approaches. At the same time, field campaigns must account for practical constraints: calibration must be conducted close to the measurement period, under similar environmental conditions, and without compromising the time allocated for actual data collection. Striking a balance between statistical robustness and operational feasibility is thus essential in designing effective calibration strategies.

While Figure 5 focused on model performance during a specific week (Week 7), Figure 6 illustrates how the performance of the different regression models evolves over time.


For particulate matter, the  $R^2$  values for the GAM model drop sharply after Week 5, indicating limited robustness and a significant reduction in predictive capability over time. In contrast, MLR and RF maintain consistently high performance until around Week 8, after which a visible decrease in  $R^2$  is observed—particularly between Weeks 8 and 9. This drop suggests that, although more stable than GAM, these models also experience a decline in accuracy when applied beyond a certain temporal window from

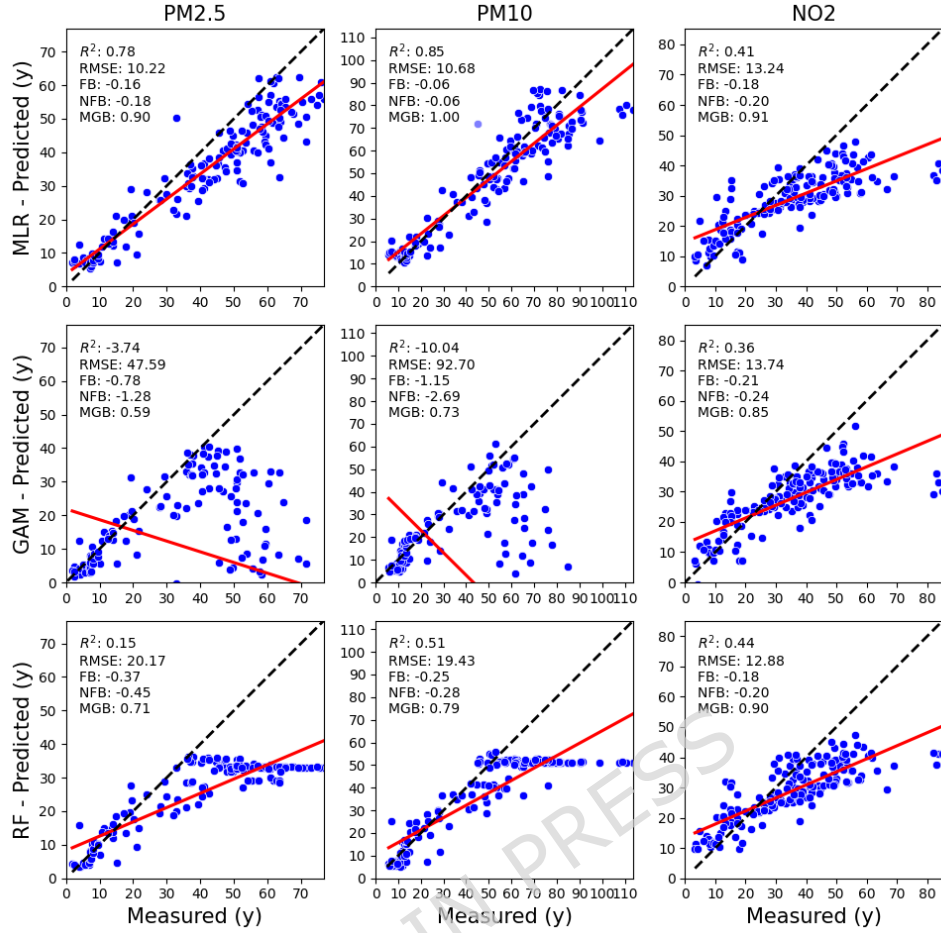

**Fig. 5** Scatter plots comparing the regression results of models trained over 2 weeks with the data measured during Week 7. Each column corresponds to a pollutant (PM<sub>2.5</sub>, PM<sub>10</sub>, NO<sub>2</sub>), each row corresponds to a statistical indicator (R<sup>2</sup>, FB, RMSE). Each point represents an hourly median concentration value, obtained by aggregating sensor measurements at hourly resolution.

the calibration period. For NO<sub>2</sub>, all three models follow a similar pattern, with R<sup>2</sup> values around 0.5 during the early weeks and a more pronounced decline after Week 8. This performance loss coincides with a one-month gap in reference data between Weeks 8 and 9 (see A) and likely reflects a temporal drift in sensor response. These findings suggest that, for all pollutants, model accuracy tends to degrade over time when applied to periods increasingly distant from the calibration, with NO<sub>2</sub> being particularly sensitive to this effect.

The RMSE trends highlight a gradual increase of error occurring immediately after the training period. For PM<sub>10</sub> and PM<sub>2.5</sub>, the error increases dramatically for the GAM model, while the MLR and the RF models maintain good performance, with

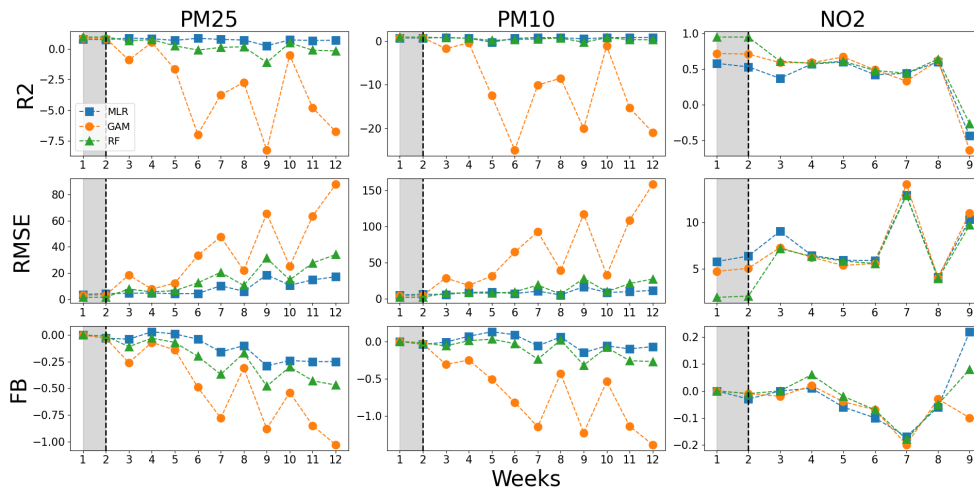

**Fig. 6** Evolution of performance metrics for the different models (MLR, GAM, and RF) considering 2 weeks of training (shaded area): calibration performance over the weeks. Each column corresponds to a pollutant (PM<sub>2.5</sub>, PM<sub>10</sub>, NO<sub>2</sub>). The three regression models—MLR, GAM, and RF—are represented by blue squares, orange circles, and green triangles, respectively. The rows display the trends for R<sup>2</sup>, RMSE, and FB over time, illustrating how model performance evolves.

MLR showing a slight advantage. Regarding NO<sub>2</sub>, the error rises after the training period, stabilizing at a plateau before a sudden increase in Week 7.

Finally, the FB provides insight into whether the low-cost sensors are underestimating (negative FB) or overestimating (positive FB) pollutant concentrations compared to reference measurements. For particulate matter, the MONICA sensors progressively underestimate concentrations over time, with the GAM model performing the worst. In the case of NO<sub>2</sub>, there is a slight overestimate in Week 4, followed by a gradual underestimate until Week 7. As highlighted also by the RMSE trends, model performance appears to improve in Week 8 (when R<sup>2</sup> also shows good values) but then deteriorates again in Week 9 (after the one-month interruption).

Overall, Figure 6 confirms that the MLR model consistently provides the most reliable results across pollutants and time, though even this model shows performance degradation when applied far from the calibration window.

The same analysis using a 3-week calibration period is provided in Appendix B, while the choice of training duration is further discussed in the following section.

### 3.3 Choice of the calibration duration

In the previous section, the performance of the regression models was analyzed using a two-week training period. This duration was selected based on a specific analysis examining how the length of the calibration phase affects the predictive accuracy of the low-cost sensors.

Figure 7 presents this analysis for the MLR model, identified as the most reliable model overall. Different markers represent the temporal evolution of model performance for varying training durations, ranging from 1 to 4 weeks. Notably, the curve corresponding to a two-week training period (orange circles) aligns with the MLR results shown in Figure 6. The training weeks were selected as the initial  $N$  weeks of the campaign to simulate a realistic deployment scenario, where a sensor is typically calibrated immediately after installation.

For all three performance metrics ( $R^2$ , RMSE, and FB), increasing the training period from one to two weeks significantly enhances the accuracy of low-cost sensor measurements for  $\text{PM}_{2.5}$  and  $\text{PM}_{10}$ . However, for  $\text{NO}_2$ , the analysis suggests that even a one-week training period is sufficient, as extending the training duration beyond that does not lead to substantial performance improvements.


This difference in optimal training duration may be explained by the representativeness of the concentration ranges encountered during the initial weeks. For  $\text{NO}_2$ , the first week alone was characterized by a high dynamic range ( $6\text{--}48\ \mu\text{g}/\text{m}^3$ ), which already covered 57% of the maximum concentration observed over the entire three-month campaign ( $85\ \mu\text{g}/\text{m}^3$ ). In contrast, for  $\text{PM}_{2.5}$  and  $\text{PM}_{10}$ , the first week captured a more limited portion of the seasonal peaks (23% and 35%, respectively). By extending the training to two weeks, these coverage percentages increased to 31% ( $40\ \mu\text{g}/\text{m}^3$ ) for  $\text{PM}_{2.5}$  and 46% ( $60\ \mu\text{g}/\text{m}^3$ ) for  $\text{PM}_{10}$ .

Compared to Figure 6, Figure 7 provides a clearer depiction of the long-term calibration stability for the MLR model, refining the findings from the previous section.

For particulate matter, both RMSE and FB show a progressive decline in performance starting from Week 6, with a more marked degradation from Week 9 onward—following the one-month interruption in the measurements. However,  $R^2$  remains relatively high even after this point (see values from Week 10 to 12). This indicates that while the model continues to capture the temporal variability and overall trends in PM concentrations (i.e., good correlation), it progressively diverges in terms of absolute values—resulting in increased bias and error. In other words, the model maintains its ability to follow the shape of the time series, but its accuracy in estimating the actual concentration levels decreases over time.

In contrast, the performance for  $\text{NO}_2$  does not exhibit a consistent trend but shows a localized increase in error and bias in Week 7, and a sharp drop in all the three statistics in Week 9—after the one-month interruption. This may indicate a shift in the underlying pollutant dynamics that is not accounted for by the initial calibration, highlighting the need for more frequent recalibration in the case of  $\text{NO}_2$ , a reactive gas with greater temporal variability.

Overall, this analysis suggests that the long-term stability of calibration models can vary significantly across pollutants and performance metrics. While the MLR model maintains good correlation with reference data over time—particularly for particulate matter—its accuracy in predicting absolute concentrations tends to deteriorate. For  $\text{NO}_2$ , calibration stability is more sensitive to time and environmental variability, indicating the need for more frequent recalibration to ensure reliable performance.

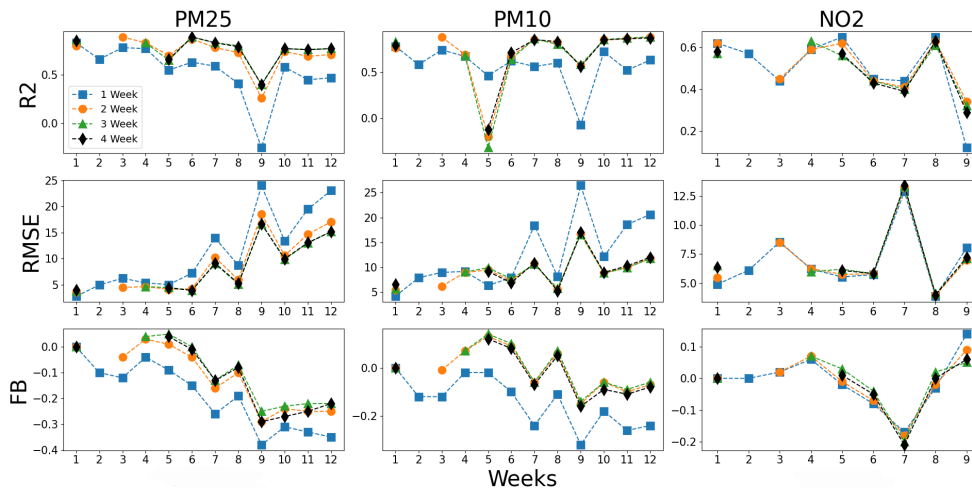

**Fig. 7** Evolution of performance metrics for MLR model considering different weeks as training: effect of calibration duration on performance. Each column corresponds to a pollutant (PM<sub>2.5</sub>, PM<sub>10</sub>, NO<sub>2</sub>), each row corresponds to a statistical indicator (R<sup>2</sup>, FB, RMSE). Each panel represents the trend of the statistical indicator over the weeks for each model used.

This sensitivity is closely linked to the seasonal variability of pollutants and meteorological drivers. The performance degradation observed after the one-month interruption suggests that short-term training may not fully capture the shifts in chemical and physical dynamics that emerge as seasonal patterns evolve.

### 3.4 Daily concentration trends and regulatory threshold analysis

After identifying the most suitable regression model (i.e., MLR), determining the optimal calibration duration (i.e., two weeks), and evaluating its long-term performance, we examined the temporal evolution of daily-averaged concentrations for PM<sub>2.5</sub> (Figure 8), PM<sub>10</sub> (Figure 9), and NO<sub>2</sub> (Figure 10). This analysis is particularly relevant in light of the new Directive (EU) 2024/2881, which introduces stricter daily (24-hour) limit values compared to previous legislation. Specifically, a new daily threshold of 50  $\mu\text{g}/\text{m}^3$  is established for NO<sub>2</sub> (not to be exceeded more than 18 times per calendar year), whereas the previous directive focused primarily on hourly peaks. Regarding particulate matter, the daily limit for PM<sub>10</sub> has been reduced from 50  $\mu\text{g}/\text{m}^3$  to 45  $\mu\text{g}/\text{m}^3$ , and the allowed number of annual exceedances has been halved from 35 to 18. Additionally, for PM<sub>2.5</sub>, a daily limit of 25  $\mu\text{g}/\text{m}^3$  has been introduced (not to be exceeded more than 18 times per year)—a parameter that was not strictly regulated in the 2008/50/EC Directive. These changes reflect a more rigorous approach to urban air quality management.

Figures 8–10 illustrate the daily-averaged concentrations for PM<sub>2.5</sub>, PM<sub>10</sub>, and NO<sub>2</sub> throughout the campaign, with the interruption period of the measurements indicated by two wavy vertical lines. For each pollutant, the plots indicate the relevant

daily concentration limits set by the new EU Directive. In addition to pollutant concentrations, the figures also display the trend of relative humidity, the only meteorological variable found to significantly contribute to the site-specific calibration models (see section 2.3).

Figure 8 illustrates the progressive increase in  $\text{PM}_{2.5}$  concentrations throughout the winter period. Measurements from the MONICA sensors show good agreement with those from the reference instruments. As previously discussed, a gradual divergence between the two datasets is observed, likely due to the progressive degradation of calibration performance. Multiple exceedances of the  $25 \mu\text{g}/\text{m}^3$  daily concentration limit, as established by Directive (EU) 2024/2881, are recorded.

The agreement between MONICA and reference instruments is even more consistent for  $\text{PM}_{10}$  (Figure 9), reflecting the slightly lower RMSE and FB values obtained for  $\text{PM}_{10}$  compared to  $\text{PM}_{2.5}$  (see Figure 7). The temporal trends of  $\text{PM}_{10}$  and  $\text{PM}_{2.5}$  are closely aligned. Notably, exceedances of the  $45 \mu\text{g}/\text{m}^3$  daily limit are frequent starting from the second week of December.


In Figure 10, MONICA sensors demonstrate a strong ability to replicate both the temporal dynamics and concentration levels of  $\text{NO}_2$ . However, a systematic underestimation of extreme values—both peaks and troughs—is evident. Notably, a significant underestimation occurs between 16 and 20 December (Week 7). This period is marked by a peak in RMSE and a negative FB, as shown in Figure 6. After the interruption period, while  $R^2$  in Figure 6 shows a significant decline for Week 9, a clear decrease in correlation is not evident in the time series data. Similar to particulate matter,  $\text{NO}_2$  levels increase over the study period, peaking in early February, a trend that is well captured by the low-cost sensor. However, unlike PM,  $\text{NO}_2$  concentrations exceed the regulatory threshold of  $50 \mu\text{g}/\text{m}^3$  only once throughout the entire period.

As a complementary analysis, Appendix B reports the same temporal trends of Figures 8-10 using a three-week calibration period. However, no substantial differences were observed compared to the two-week calibration, confirming its adequacy for this application.


Table 4 summarizes the number of exceedances for each pollutant, based on the daily thresholds set by Directive (EU) 2024/2881. The number of exceedances estimated by MONICA (two-weeks training) is almost identical to that recorded by reference instrumentation, underscoring the potential of low-cost sensors for regulatory monitoring purposes. Notably, the daily limit for  $\text{PM}_{2.5}$  is exceeded on more than 60% of the days in the observation period, approximately 40% for  $\text{PM}_{10}$ , and around 2% for  $\text{NO}_2$ . Directive (EU) 2024/2881 allows a maximum of 18 exceedances per year for each pollutant; this threshold is significantly surpassed in our dataset, despite the dataset spanning slightly more than three months.

Table 4 also includes the average concentrations for each pollutant over the measurement period. As expected, given the predominantly negative fractional bias values reported earlier, the MONICA sensors tend to underestimate concentrations by approximately 18% for  $\text{PM}_{2.5}$ , 13% for  $\text{PM}_{10}$ , and 1% for  $\text{NO}_2$ . It is worth noting that the average  $\text{PM}_{2.5}$  concentration measured during the campaign exceeds the current annual limit of  $10 \mu\text{g}/\text{m}^3$  set by Directive (EU) 2024/2881. A similar pattern is observed for  $\text{PM}_{10}$ , whose reference average of  $42.43 \mu\text{g}/\text{m}^3$  exceeds both


the current (European Directive 2008/50/CE [78]) annual limit of  $40 \mu\text{g}/\text{m}^3$  and the upcoming  $20 \mu\text{g}/\text{m}^3$  limit. For  $\text{NO}_2$ , only the newly introduced annual limit of  $20 \mu\text{g}/\text{m}^3$  is exceeded. In performing these comparison, it is worth remembering that the measurements reported here refer only to the winter season, during which meteorological conditions (and increased pollutant emissions, notably due to domestic heating) typically lead to the highest pollutant levels observed over the whole year.

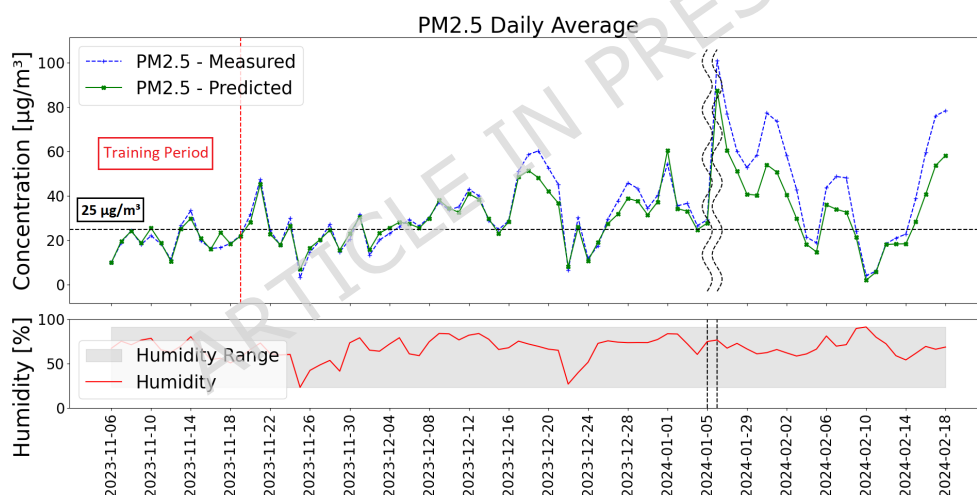

**Fig. 8** Comparison of daily average  $\text{PM}_{2.5}$  concentrations measured by the reference instrument (dashed blue line) and those estimated by MONICA (green line) using the MLR regression model trained over a two-week period. The regulatory limit established by Directive (EU) 2024/2881 is shown as a dashed horizontal line. The trend of relative humidity is also reported (red line). The measurement interruption period is indicated by vertical dashed lines.

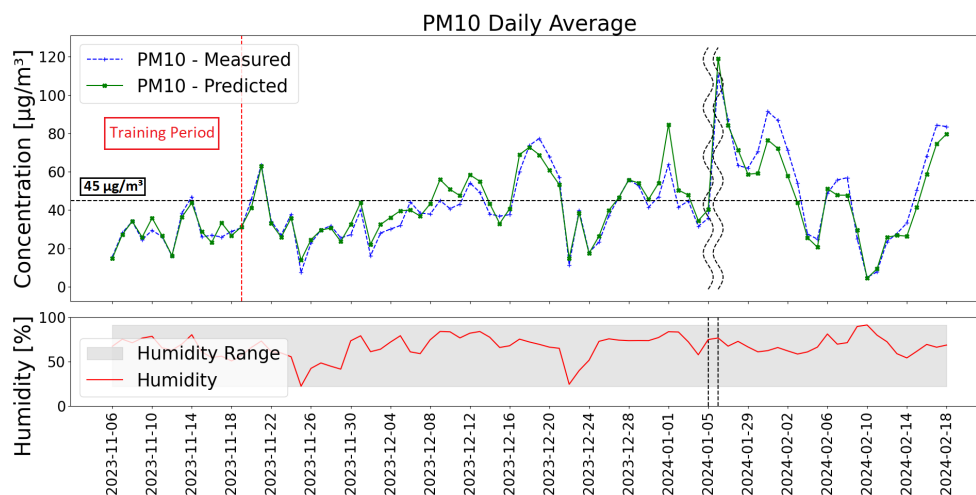

**Fig. 9** Comparison of daily average  $\text{PM}_{10}$  concentrations measured by the reference instrument (dashed blue line) and those estimated by MONICA (green line) using the MLR regression model trained over a two-week period. The regulatory limit established by Directive (EU) 2024/2881 is shown as a dashed horizontal line. The trend of relative humidity is also reported (red line). The measurement interruption period is indicated by vertical dashed lines.

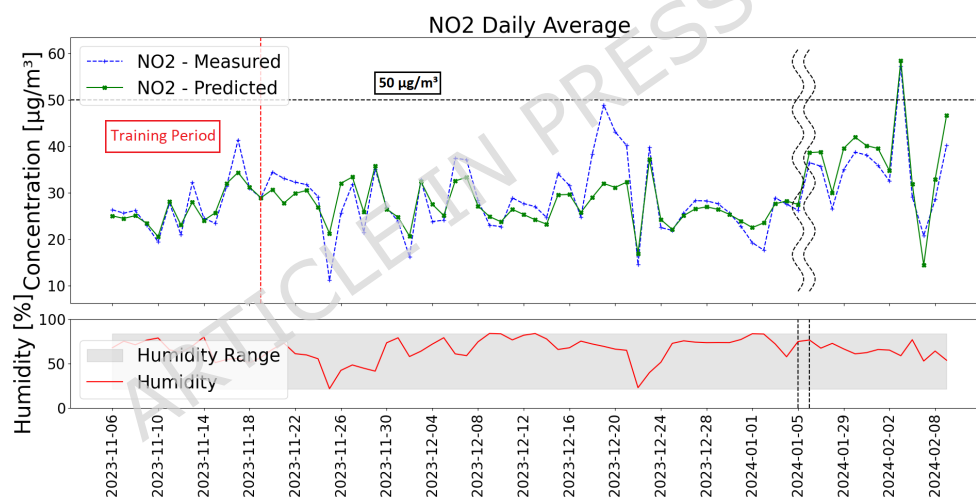

**Fig. 10** Comparison of daily average  $\text{NO}_2$  concentrations measured by the reference instrument (dashed blue line) and those estimated by MONICA (green line) using the MLR regression model trained over a two-week period. The regulatory limit established by Directive (EU) 2024/2881 is shown as a dashed horizontal line. The trend of relative humidity is also reported (red line). The measurement interruption period is indicated by vertical dashed lines.

**Table 4** Number of exceedances based on the daily limits established by European Directive (EU) 2024/2881, as estimated over a 12-week measurement period for particulate matter (PM<sub>10</sub> and PM<sub>2.5</sub>) and a 9-week measurement period for NO<sub>2</sub>, along with average concentrations over the entire period for each pollutant.

| Instrument  | Exceedances [#]             |                             |                             | Average Concentration      |                            |                            |
|-------------|-----------------------------|-----------------------------|-----------------------------|----------------------------|----------------------------|----------------------------|
|             | PM <sub>2.5</sub>           | PM <sub>10</sub>            | NO <sub>2</sub>             | PM <sub>2.5</sub>          | PM <sub>10</sub>           | NO <sub>2</sub>            |
|             | 25 $\mu\text{g}/\text{m}^3$ | 45 $\mu\text{g}/\text{m}^3$ | 50 $\mu\text{g}/\text{m}^3$ | $[\mu\text{g}/\text{m}^3]$ | $[\mu\text{g}/\text{m}^3]$ | $[\mu\text{g}/\text{m}^3]$ |
| Ref. Instr. | 51                          | 31                          | 1                           | 33.90                      | 42.43                      | 29.26                      |
| MONICA      | 50                          | 33                          | 1                           | 27.90                      | 36.81                      | 29.02                      |

## 4 Conclusions

This study evaluated the performance and calibration strategies of the MONICA low-cost sensor system for measuring particulate matter (PM<sub>2.5</sub> and PM<sub>10</sub>) and nitrogen dioxide (NO<sub>2</sub>) in an urban setting. Our primary objective was to identify the most reliable calibration model, assess the optimal co-location duration, and analyze the long-term stability of sensor performance.

Among the models tested, Multiple Linear Regression (MLR) proved to be significantly more robust than both the Generalized Additive Model (GAM) and Random Forest (RF) models. The latter models exhibited high sensitivity to the dataset used for calibration and struggled to predict the highest concentration values accurately.

In terms of calibration duration, our analysis revealed that a two-week calibration period was sufficient for particulate matter, providing reliable sensor performance for up to seven weeks post-calibration. For NO<sub>2</sub>, however, a shorter, one-week calibration period proved to be adequate, as extending the duration beyond that did not result in significant performance improvements. This suggests that the calibration duration can vary depending on the pollutant and, more importantly, on the environmental representativeness of the training window. In our study, the high urban variability allowed the sensors to encounter a significant portion of the seasonal dynamic range (covering up to 57% of the campaign maximum for NO<sub>2</sub> in the first week, and 46% for PM<sub>10</sub> by the second) within these short timeframes. This ensured that the models were well-constrained from the outset for the specific conditions of the monitored period.

The long-term evaluation revealed important differences in sensor behavior. While PM sensors maintained a good correlation with reference data over time, their accuracy in predicting absolute concentrations declined gradually, as reflected in increasing RMSE and fractional bias. For NO<sub>2</sub>, a more abrupt degradation was observed, especially after two months, suggesting a higher susceptibility to sensor drift and environmental variability. This degradation also reflects the inherent seasonal limitations of the study; while the models included parameters to compensate for ozone interference, the narrow range of conditions typical of a winter campaign may limit their applicability to summer months, when higher ozone levels and broader temperature fluctuations occur. A general tendency toward underestimation was found for all pollutants, reinforcing the need for regular validation against reference-grade instruments.

639 Despite these limitations, MONICA sensors successfully captured temporal trends  
640 and regulatory exceedances, confirming their suitability for urban air quality surveil-  
641 lance and public health applications. Their affordability, compact design, and accept-  
642 able long-term performance make them attractive tools for enhancing spatial and  
643 temporal resolution in monitoring networks.

644 In summary, this study demonstrates that low-cost multi-pollutant systems like  
645 MONICA can deliver reliable results over extended periods, provided that calibra-  
646 tion strategies are carefully designed and periodically updated. The findings provide  
647 operational guidance for optimizing sensor deployments under real-world constraints,  
648 contributing to the development of scalable and cost-effective air quality networks.

649 Future work should explore multi-seasonal deployments, longer observation peri-  
650 ods, and parallel sensor configurations to evaluate spatial variability and further refine  
651 calibration methods. Integrating these insights into policy and urban planning could  
652 enhance the responsiveness and equity of air quality management strategies.

## A Time windows with valid data for calibration and evaluation

The monitoring campaign took place from November 6, 2023, to February 25, 2024, with MONICA sensors co-located alongside reference instruments. Due to interruptions in the reference instruments, the time windows with valid data for direct comparison were limited: 12 full weeks for PM<sub>2.5</sub> and PM<sub>10</sub>, and 9 full weeks for NO<sub>2</sub>. Table A.1 indicates the weeks with complete data coverage as well as those with partial or no data.


**Table A1** Availability of valid data for PM<sub>2.5</sub>, PM<sub>10</sub>, and NO<sub>2</sub>, broken down by full weeks (Monday to Sunday). Only weeks with complete data coverage are numbered.

| Week    | Date Range           | Available Pollutants                                                       |
|---------|----------------------|----------------------------------------------------------------------------|
| Week 1  | 06–12 Nov 2023       | PM <sub>2.5</sub> , PM <sub>10</sub> , NO <sub>2</sub>                     |
| Week 2  | 13–19 Nov 2023       | PM <sub>2.5</sub> , PM <sub>10</sub> , NO <sub>2</sub>                     |
| Week 3  | 20–26 Nov 2023       | PM <sub>2.5</sub> , PM <sub>10</sub> , NO <sub>2</sub>                     |
| Week 4  | 27 Nov – 03 Dec 2023 | PM <sub>2.5</sub> , PM <sub>10</sub> , NO <sub>2</sub>                     |
| Week 5  | 04–10 Dec 2023       | PM <sub>2.5</sub> , PM <sub>10</sub> , NO <sub>2</sub>                     |
| Week 6  | 11–17 Dec 2023       | PM <sub>2.5</sub> , PM <sub>10</sub> , NO <sub>2</sub>                     |
| Week 7  | 18–24 Dec 2023       | PM <sub>2.5</sub> , PM <sub>10</sub> , NO <sub>2</sub>                     |
| Week 8  | 25–31 Dec 2023       | PM <sub>2.5</sub> , PM <sub>10</sub> , NO <sub>2</sub>                     |
| –       | 01–07 Jan 2024       | PM <sub>2.5</sub> , PM <sub>10</sub> , NO <sub>2</sub> (only until 05 Jan) |
| –       | 08–14 Jan 2024       | No data                                                                    |
| –       | 15–21 Jan 2024       | No data                                                                    |
| –       | 22–28 Jan 2024       | PM <sub>2.5</sub> , PM <sub>10</sub> , NO <sub>2</sub> (starting 25 Jan)   |
| Week 9  | 29 Jan – 04 Feb 2024 | PM <sub>2.5</sub> , PM <sub>10</sub> , NO <sub>2</sub>                     |
| Week 10 | 05–11 Feb 2024       | PM <sub>2.5</sub> , PM <sub>10</sub>                                       |
| Week 11 | 12–18 Feb 2024       | PM <sub>2.5</sub> , PM <sub>10</sub>                                       |
| Week 12 | 19–25 Feb 2024       | PM <sub>2.5</sub> , PM <sub>10</sub>                                       |


## B Results for 3-weeks training

The comparison of three regression models and the analysis of their performance relative to the training period indicated that a 2-week training period for the MLR model offers the optimal balance for real-world campaigns conducted within a single season. In this appendix, we present the comparison between MONICA measurements and those from the reference instruments using a 3-week training period for the MLR model.


Figures A3 to A2 show that a 3-week training period yields results that are practically identical to those observed in Figures 10 to 9, confirming that a 2-week period is sufficient and optimal for calibration.

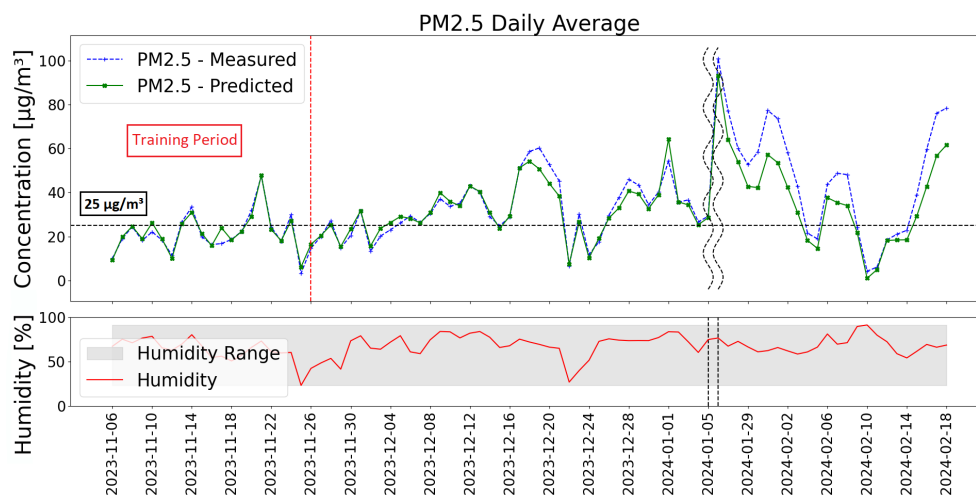

**Fig. A1** Comparison of daily average  $\text{PM}_{2.5}$  concentrations measured by the reference instrument (dashed blue line) and those estimated by MONICA (green line) using the MLR regression model trained over a three-week period. The regulatory limit established by Directive (EU) 2024/2881 is shown as a dashed horizontal line. The trend of relative humidity is also reported (red line). The measurement interruption period is indicated by vertical dashed lines.

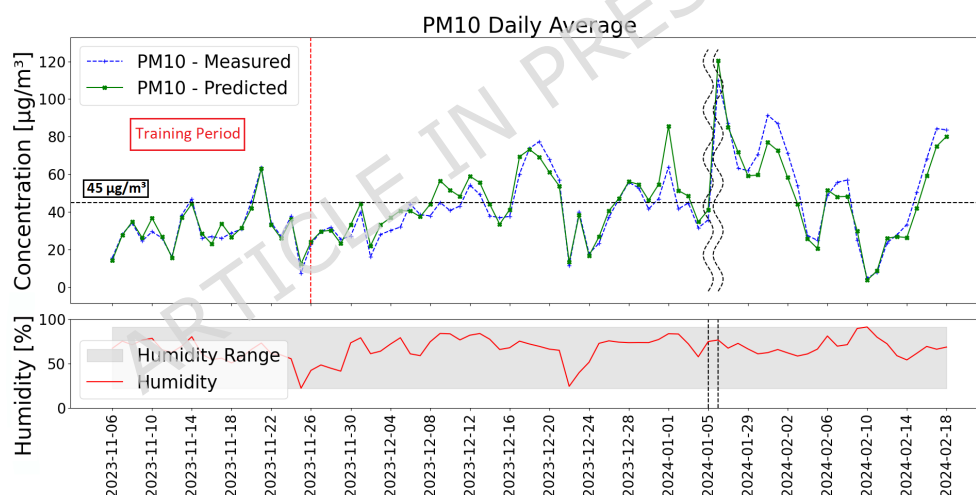

**Fig. A2** Comparison of daily average  $\text{PM}_{10}$  concentrations measured by the reference instrument (dashed blue line) and those estimated by MONICA (green line) using the MLR regression model trained over a three-week period. The regulatory limit established by Directive (EU) 2024/2881 is shown as a dashed horizontal line. The trend of relative humidity is also reported (red line). The measurement interruption period is indicated by vertical dashed lines.

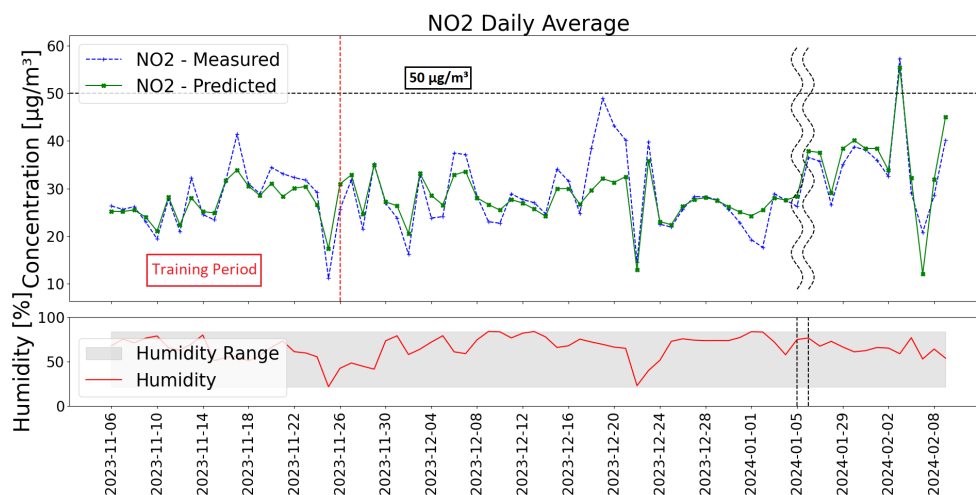

**Fig. A3** Comparison of daily average  $\text{NO}_2$  concentrations measured by the reference instrument (dashed blue line) and those estimated by MONICA (green line) using the MLR regression model trained over a three-week period. The regulatory limit established by Directive (EU) 2024/2881 is shown as a dashed horizontal line. The trend of relative humidity is also reported (red line). The measurement interruption period is indicated by vertical dashed lines.

## Declarations

## Consent for Participation and Publication

Not applicable.

## Availability of data and materials

The dataset generated and analyzed during the current study, including raw low-cost sensor outputs and reference instrument data, is provided as Supplementary Material to ensure the transparency and reproducibility of the results.

## Competing interests

The authors have no relevant financial or non-financial interests to disclose. The authors declare that they have no conflict of interest.

## Funding

The authors did not receive any specific grant from funding agencies in the public, commercial, or not-for-profit sectors for the research, authorship, and/or publication of this article.

## Authors' contributions

S.F. conceptualized the study, developed the methodology, and wrote the original draft. D.G. curated data, created visualizations, and contributed to writing the original draft. V.V. performed formal analysis, created visualizations, and contributed to writing the original draft. N.M. curated data and helped review the manuscript. G.F. provided resources. M.C. conceptualized the study, supervised and managed the project, reviewed the manuscript. P.S. conceptualized the study, supervised the work, reviewed the manuscript, and managed the project.

## Acknowledgments

This work was conducted within the climate\_transition@polito project, funded by the Italian Ministry of University and Research under the 2023–2027 “Departments of Excellence” program. The authors thank Gerardo D’Elia, Saverio De Vito, and Sergio Ferlito (ENEA – Portici Research Center) for their technical support and collaboration. P.S. acknowledges funding from the Auvergne-Rhône-Alpes Region through the VEB<sub>MU</sub> project. S.F. and M.C. acknowledge funding from Fondazione Compagnia di San Paolo through the LIBRA project.

## References

- [1] Di, Q., Dai, L., Wang, Y., Zanobetti, A., Choirat, C., Schwartz, J.D., Dominici, F.: Association of short-term exposure to air pollution with mortality in older adults. *Jama* **318**(24), 2446–2456 (2017)
- [2] Hystad, P., Larkin, A., Rangarajan, S., AlHabib, K.F., Avezum, Á., Calik, K.B.T., Chifamba, J., Dans, A., Diaz, R., Du Plessis, J.L., *et al.*: Associations of outdoor fine particulate air pollution and cardiovascular disease in 157 436 individuals from 21 high-income, middle-income, and low-income countries (pure): a prospective cohort study. *The Lancet Planetary Health* **4**(6), 235–245 (2020)
- [3] Lin, C.-K., Chang, Y.-T., Lee, F.-S., Chen, S.-T., Christiani, D.: Association between exposure to ambient particulate matters and risks of autism spectrum disorder in children: a systematic review and exposure-response meta-analysis. *Environmental Research Letters* **16**(6), 063003 (2021)
- [4] De Bont, J., Krishna, B., Stafoggia, M., Banerjee, T., Dholakia, H., Garg, A., Ingole, V., Jaganathan, S., Kloog, I., Lane, K., *et al.*: Ambient air pollution and daily mortality in ten cities of india: a causal modelling study. *The Lancet Planetary Health* **8**(7), 433–440 (2024)
- [5] Salizzoni, P., Soulhac, L., Mejean, P.: Street canyon ventilation and atmospheric turbulence. *Atmospheric Environment* **43**(32), 5056–5067 (2009)
- [6] Fellini, S., Salizzoni, P., Ridolfi, L.: Vulnerability of cities to toxic airborne releases is written in their topology. *Scientific Reports* **11**(1), 23029 (2021)

- 722 [7] Kim, K.-H., Kabir, E., Kabir, S.: A review on the human health impact of airborne  
723 particulate matter **74**, 136–143 (2015) <https://doi.org/10.1016/j.envint.2014.10.005> . Accessed 2024-09-26  
724
- 725 [8] Chen, J., Hoek, G.: Long-term exposure to PM and all-cause and cause-specific  
726 mortality: A systematic review and meta-analysis **143**, 105974 (2020) <https://doi.org/10.1016/j.envint.2020.105974> . Accessed 2024-09-26  
727
- 728 [9] Kang, J., Choi, K.: Calibration methods for low-cost particulate matter sen-  
729 sors considering seasonal variability **24**(10), 3023 (2024) <https://doi.org/10.3390/s24103023> . Accessed 2024-09-26  
730
- 731 [10] Pope, C.A., Dockery, D.W.: Health effects of fine particulate air pollution: lines  
732 that connect. *Journal of the air & waste management association* **56**(6), 709–742  
733 (2006)
- 734 [11] WHO: Review of evidence on health aspects of air pollution: Revihaap project:  
735 technical report. In: *Review of Evidence on Health Aspects of Air Pollution: REVIHAAP Project: Technical Report*, (2021)  
736
- 737 [12] Khreis, H., Kelly, C., Tate, J., Parslow, R., Lucas, K., Nieuwenhuijsen, M.: Expo-  
738 sure to traffic-related air pollution and risk of development of childhood asthma:  
739 a systematic review and meta-analysis. *Environment international* **100**, 1–31  
740 (2017)
- 741 [13] Anenberg, S.C., Mohegh, A., Goldberg, D.L., Kerr, G.H., Brauer, M., Burkart,  
742 K., Hystad, P., Larkin, A., Wozniak, S., Lamsal, L.: Long-term trends in urban  
743 *no<sub>2</sub>* concentrations and associated paediatric asthma incidence: estimates from  
744 global datasets. *The Lancet Planetary Health* **6**(1), 49–58 (2022)
- 745 [14] Soulhac, L., Fellini, S., Nguyen, C.V., Salizzoni, P.: Evaluation of photostationary  
746 and non-photostationary operational models for *nox* pollution in a street canyon.  
747 *Atmospheric Environment* **297**, 119589 (2023)
- 748 [15] European Parliament and Council: Directive (EU) 2024/2881 of the European  
749 Parliament and of the Council of 23 October 2024 on ambient air quality and  
750 cleaner air for Europe.  
751 <https://eur-lex.europa.eu/eli/dir/2024/2881/oj/eng> (2024)
- 752 [16] Steinle, S., Reis, S., Sabel, C.E., Semple, S., Twigg, M.M., Braban, C.F., Leeson,  
753 S.R., Heal, M.R., Harrison, D., Lin, C., Wu, H.: Personal exposure monitoring  
754 of PM 2.5 in indoor and outdoor microenvironments **508**, 383–394 (2015) <https://doi.org/10.1016/j.scitotenv.2014.12.003> . Accessed 2024-11-04  
755
- 756 [17] Fellini, S., Salizzoni, P., Ridolfi, L.: Effect of emission variability on concentration  
757 fluctuations in idealised deep urban street canyons. *Urban Climate* **55**, 101952  
758 (2024)

- [18] McHugh, C., Carruthers, D., Edmunds, H.: ADMS–Urban: an air quality management system for traffic, domestic and industrial pollution. *International Journal of Environment and Pollution* **8**(3-6), 666–674 (1997)
- [19] Soulhac, L., Salizzoni, P., Cierco, F., Perkins, R.: The model SIRANE for atmospheric urban pollutant dispersion; part i, presentation of the model. *Atmospheric environment* **45**(39), 7379–7395 (2011)
- [20] Kim, Y., Wu, Y., Seigneur, C., Roustan, Y.: Multi-scale modeling of urban air pollution: development and application of a street-in-grid model (v1. 0) by coupling munich (v1. 0) and polair3d (v1. 8.1). *Geoscientific Model Development* **11**(2), 611–629 (2018)
- [21] Suter, I., Grylls, T., Sützl, B., Reeuwijk, M.: udales 1.0. 0: a large-eddy-simulation model for urban environments. *Geoscientific Model Development Discussions* **2021**, 1–40 (2021)
- [22] Hoek, G., Beelen, R., De Hoogh, K., Vienneau, D., Gulliver, J., Fischer, P., Briggs, D.: A review of land-use regression models to assess spatial variation of outdoor air pollution. *Atmospheric environment* **42**(33), 7561–7578 (2008)
- [23] Beelen, R., Hoek, G., Vienneau, D., Eeftens, M., Dimakopoulou, K., Pedeli, X., Tsai, M.-Y., Künzli, N., Schikowski, T., Marcon, A., *et al.*: Development of no<sub>2</sub> and nox land use regression models for estimating air pollution exposure in 36 study areas in europe—the escape project. *Atmospheric Environment* **72**, 10–23 (2013)
- [24] Ma, X., Zou, B., Deng, J., Gao, J., Longley, I., Xiao, S., Guo, B., Wu, Y., Xu, T., Xu, X., *et al.*: A comprehensive review of the development of land use regression approaches for modeling spatiotemporal variations of ambient air pollution: A perspective from 2011 to 2023. *Environment international* **183**, 108430 (2024)
- [25] Liu, S., Tian, H., Luo, L., Bai, X., Zhu, C., Lin, S., Zhao, S., Zhang, K., Hao, J., Guo, Z., Lv, Y.: Health impacts and spatiotemporal variations of fine particulate and its typical toxic constituents in five urban agglomerations of China. *Science of The Total Environment* **806**, 151459 (2022) <https://doi.org/10.1016/j.scitotenv.2021.151459> . Accessed 2024-12-16
- [26] Schmitz, S., Caseiro, A., Kerschbaumer, A., Von Schneidemesser, E.: Quantifying impacts of local traffic policies on PM concentrations using low cost sensors in berlin **24**(9), 240050 (2024) <https://doi.org/10.4209/aaqr.240050> . Accessed 2024-09-26
- [27] Tang, H., Cai, Y., Gao, S., Sun, J., Ning, Z., Yu, Z., Pan, J., Zhao, Z.: Multi-scenario validation and assessment of a particulate matter sensor monitor optimized by machine learning methods **24**(11), 3448 (2024) <https://doi.org/10.3390/s24113448> . Accessed 2024-09-25

- [28] Cross, E.S., Williams, L.R., Lewis, D.K., Magoon, G.R., Onasch, T.B., Kaminsky, M.L., Worsnop, D.R., Jayne, J.T.: Use of electrochemical sensors for measurement of air pollution: correcting interference response and validating measurements. *Atmospheric Measurement Techniques* **10**(9), 3575–3588 (2017) <https://doi.org/10.5194/amt-10-3575-2017>
- [29] Thomas, G.W., Sousan, S., Tatum, M., Liu, X., Zuidema, C., Fitzpatrick, M., Koehler, K.A., Peters, T.M.: Low-Cost, Distributed Environmental Monitors for Factory Worker Health. *Sensors* **18**(5), 1411 (2018) <https://doi.org/10.3390/s18051411> . Accessed 2024-12-09
- [30] Johnson, K.K., Bergin, M.H., Russell, A.G., Hagler, G.S.W.: Field Test of Several Low-Cost Particulate Matter Sensors in High and Low Concentration Urban Environments. *Aerosol and Air Quality Research* **18**(3), 565–578 (2018) <https://doi.org/10.4209/aaqr.2017.10.0418> . Accessed 2024-12-09
- [31] Hagan, D.H., Isaacman-VanWertz, G., Franklin, J.P., Wallace, L.M.M., Kocar, B.D., Heald, C.L., Kroll, J.H.: Calibration and assessment of electrochemical air quality sensors by co-location with regulatory-grade instruments. *Atmospheric Measurement Techniques* **11**(1), 315–328 (2018) <https://doi.org/10.5194/amt-11-315-2018>
- [32] Badura, M., Batog, P., Drzeniecka-Osiadacz, A., Modzel, P.: Evaluation of low-cost sensors for ambient pm2.5 monitoring. *Journal of Sensors* **2018**(1), 5096540 (2018) <https://doi.org/10.1155/2018/5096540> <https://onlinelibrary.wiley.com/doi/pdf/10.1155/2018/5096540>
- [33] Cavaliere, A., Carotenuto, F., Di Gennaro, F., Gioi, B., Gualtieri, G., Martelli, F., Matese, A., Toscano, P., Vagnoli, C., Zaldei, A.: Development of low-cost air quality stations for next generation monitoring networks: Calibration and validation of pm2.5 and pm10 sensors. *Sensors* **18**(9) (2018) <https://doi.org/10.3390/s18092843>
- [34] Wang, Y., Li, J., Jing, H., Zhang, Q., Jiang, J., Biswas, P.: Laboratory evaluation and calibration of three low-cost particle sensors for particulate matter measurement. *Aerosol science and technology* **49**(11), 1063–1077 (2015)
- [35] Bulot, F.M.J., Johnston, S.J., Basford, P.J., Easton, N.H.C., Apetroaie-Cristea, M., Foster, G.L., Morris, A.K.R., Cox, S.J., Loxham, M.: Long-term field comparison of multiple low-cost particulate matter sensors in an outdoor urban environment. *Scientific Reports* **9**(1), 7497 (2019) <https://doi.org/10.1038/s41598-019-43716-3> . Accessed 2024-12-09
- [36] Giordano, M.R., Malings, C., Pandis, S.N., Presto, A.A., McNeill, V.F., Westervelt, D.M., Beekmann, M., Subramanian, R.: From low-cost sensors to high-quality data: A summary of challenges and best practices for effectively calibrating low-cost particulate matter mass sensors **158**, 105833 (2021) <https://doi.org/10.1016/j.atmosenv.2021.105833>

- 1016/j.jaerosci.2021.105833 . Accessed 2024-09-25
- [37] Venkatraman Jagatha, J., Klausnitzer, A., Chacón-Mateos, M., Laquai, B., Nieuwkoop, E., Van Der Mark, P., Vogt, U., Schneider, C.: Calibration Method for Particulate Matter Low-Cost Sensors Used in Ambient Air Quality Monitoring and Research. *Sensors* **21**(12), 3960 (2021) <https://doi.org/10.3390/s21123960> . Accessed 2025-01-27
- [38] Zimmerman, N.: Tutorial: Guidelines for implementing low-cost sensor networks for aerosol monitoring **159**, 105872 (2022) <https://doi.org/10.1016/j.jaerosci.2021.105872> . Accessed 2024-09-25
- [39] Crilley, L.R., Shaw, M., Pound, R., Kramer, L.J., Price, R., Young, S., Lewis, A.C., Pope, F.D.: Evaluation of a low-cost optical particle counter (alphasense opc-n2) for ambient air monitoring. *Atmospheric Measurement Techniques* **11**(2), 709–720 (2018) <https://doi.org/10.5194/amt-11-709-2018>
- [40] Di Antonio, A., Popoola, O.A.M., Ouyang, B., Saffell, J., Jones, R.L.: Developing a Relative Humidity Correction for Low-Cost Sensors Measuring Ambient Particulate Matter. *Sensors* **18**(9), 2790 (2018) <https://doi.org/10.3390/s18092790> . Accessed 2025-01-30
- [41] Macías-Hernández, B.A., Tello-Leal, E., Barrios S., O., Leiva-Guzmán, M.A., Toro A., R.: Effect of environmental conditions on the performance of a low-cost atmospheric particulate matter sensor **52**, 101753 (2023) <https://doi.org/10.1016/j.uclim.2023.101753> . Accessed 2024-11-04
- [42] Datta, A., Saha, A., Zamora, M.L., Buehler, C., Hao, L., Xiong, F., Gentner, D.R., Koehler, K.: Statistical field calibration of a low-cost PM<sub>2.5</sub> monitoring network in Baltimore. *Atmospheric Environment* **242**, 117761 (2020) <https://doi.org/10.1016/j.atmosenv.2020.117761> . Accessed 2025-01-30
- [43] Jiao, W., Hagler, G., Williams, R., Sharpe, R., Brown, R., Garver, D., Judge, R., Caudill, M., Rickard, J., Davis, M., Weinstock, L., Zimmer-Dauphinee, S., Buckley, K.: Community air sensor network (cairsense) project: evaluation of low-cost sensor performance in a suburban environment in the southeastern united states. *Atmospheric Measurement Techniques* **9**(11), 5281–5292 (2016) <https://doi.org/10.5194/amt-9-5281-2016>
- [44] Mijling, B., Jiang, Q., De Jonge, D., Bocconi, S.: Field calibration of electrochemical NO<sub>2</sub> sensors in a citizen science context. *Atmospheric Measurement Techniques* **11**(3), 1297–1312 (2018) <https://doi.org/10.5194/amt-11-1297-2018> . Accessed 2025-02-12
- [45] Ratingen, S.V., Vonk, J., Blokhuis, C., Wesseling, J., Tielemans, E., Weijers, E.: Seasonal Influence on the Performance of Low-Cost NO<sub>2</sub> Sensor Calibrations.

- 873 Sensors **21**(23), 7919 (2021) <https://doi.org/10.3390/s21237919> . Accessed 2025-  
874 02-12
- 875 [46] Nowack, P., Konstantinovskiy, L., Gardiner, H., Cant, J.: Machine learning cali-  
876 bration of low-cost NO<sub>2</sub> and PM<sub>10</sub> sensors: non-linear algorithms and their impact  
877 on site transferability. *Atmospheric Measurement Techniques* **14**(8), 5637–5655  
878 (2021) <https://doi.org/10.5194/amt-14-5637-2021> . Accessed 2025-02-12
- 879 [47] Kim, H., Müller, M., Henne, S., Hüglin, C.: Long-term behavior and stabil-  
880 ity of calibration models for NO and NO<sub>2</sub> low cost sensors (2022). <https://doi.org/10.5194/amt-2021-433> . [https://amt.copernicus.org/articles/15/2979/2022/](https://amt.copernicus.org/articles/15/2979/2022/amt-15-2979-2022-discussion.html)  
881 [amt-15-2979-2022-discussion.html](https://amt.copernicus.org/articles/15/2979/2022/amt-15-2979-2022-discussion.html) Accessed 2025-02-12
- 883 [48] Malings, C., Tanzer, R., Hauryliuk, A., Kumar, S.P.N., Zimmerman, N., Kara,  
884 L.B., Presto, A.A., Subramanian, R.: Development of a general calibration model  
885 and long-term performance evaluation of low-cost sensors for air pollutant gas  
886 monitoring. *Atmospheric Measurement Techniques* **12**(2), 903–920 (2019) <https://doi.org/10.5194/amt-12-903-2019>  
887
- 888 [49] Cross, E.S., Williams, L.R., Lewis, D.K., Magoon, G.R., Onasch, T.B., Kaminsky,  
889 M.L., Worsnop, D.R., Jayne, J.T.: Use of electrochemical sensors for measurement  
890 of air pollution: correcting interference response and validating measurements.  
891 *Atmospheric Measurement Techniques* **10**(9), 3575–3588 (2017)
- 892 [50] Gäbel, P., Koller, C., Hertig, E.: Development of Air Quality Boxes Based on Low-  
893 Cost Sensor Technology for Ambient Air Quality Monitoring. *Sensors* **22**(10),  
894 3830 (2022) <https://doi.org/10.3390/s22103830> . Accessed 2024-12-09
- 895 [51] Cavaliere, A., Brilli, L., Andreini, B.P., Carotenuto, F., Gioli, B., Giordano,  
896 T., Stefanelli, M., Vagnoli, C., Zaldei, A., Gualtieri, G.: Development of low-  
897 cost air quality stations for next-generation monitoring networks: calibration  
898 and validation of NO<sub>2</sub> and O<sub>3</sub> sensors. *Atmospheric Measurement Techniques*  
899 **16**(20), 4723–4740 (2023) <https://doi.org/10.5194/amt-16-4723-2023> . Accessed  
900 2025-02-12
- 901 [52] Levy Zamora, M., Buehler, C., Datta, A., Gentner, D.R., Koehler, K.: Ident-  
902 ifying optimal co-location calibration periods for low-cost sensors. *Atmo-*  
903 *spheric Measurement Techniques* **16**(1), 169–179 (2023) [https://doi.org/10.5194/](https://doi.org/10.5194/amt-16-169-2023)  
904 [amt-16-169-2023](https://doi.org/10.5194/amt-16-169-2023)
- 905 [53] De Vito, S., Esposito, E., Castell, N., Schneider, P., Bartonova, A.: On the robust-  
906 ness of field calibration for smart air quality monitors. *Sensors and Actuators B:*  
907 *Chemical* **310**, 127869 (2020) <https://doi.org/10.1016/j.snb.2020.127869>
- 908 [54] De Vito, S., Esposito, E., Massera, E., Formisano, F., Fattoruso, G., Ferlito, S.,  
909 Del Giudice, A., D’Elia, G., Salvato, M., Polichetti, T., D’Auria, P., Ionescu, A.M.,

- 910 Di Francia, G.: Crowdsensing iot architecture for pervasive air quality and expo-  
 911 some monitoring: Design, development, calibration, and long-term validation.  
 912 *Sensors* **21**(15) (2021) <https://doi.org/10.3390/s21155219>
- 913 [55] Fattoruso, G., Toscano, D., Cornelio, A., De Vito, S., Murena, F., Fabbicino, M.,  
 914 Di Francia, G.: Using mobile monitoring and atmospheric dispersion modeling  
 915 for capturing high spatial air pollutant variability in cities. *Atmosphere* **13**(11)  
 916 (2022) <https://doi.org/10.3390/atmos13111933>
- 917 [56] De Vito, S., Del Giudice, A., D'Elia, G., Esposito, E., Fattoruso, G., Ferlito, S.,  
 918 Formisano, F., Loffredo, G., Massera, E., Bellucci, P., Ciarallo, F., Di Francia,  
 919 G.: Correlating air pollution concentrations and vehicular emissions in an italian  
 920 roadway tunnel by means of low cost sensors **14**(4) (2023) <https://doi.org/10.3390/atmos14040679>  
 921
- 922 [57] Ramel-Delobel, M., Peruzzi, C., Coudon, T., De Vito, S., Fattoruso, G., Praud,  
 923 D., Fervers, B., Salizzoni, P.: Exposure to airborne particulate matter during com-  
 924 muting using portable sensors: Effects of transport modes in a french metropolis  
 925 study case **365**, 121400 (2024) <https://doi.org/10.1016/j.jenvman.2024.121400> .  
 926 Accessed 2024-09-25
- 927 [58] Bo, M., Charvolin-Volta, P., Clerico, M., Nguyen, C.V., Pognant, F., Soulhac, L.,  
 928 Salizzoni, P.: Urban air quality and meteorology on opposite sides of the alps:  
 929 The lyon and torino case studies. *Urban Climate* **34**, 100698 (2020)
- 930 [59] Beijing Plantower Co., Ltd: PMS7003 Series DataSheet - Digital Universal  
 931 Particle Concentration Sensor. [https://plantower.com/en/products\\_33/76.html](https://plantower.com/en/products_33/76.html)
- 932 [60] Alphasense - AMETEK Inc.: CO-A4 Carbon Monoxide Sensor - Datasheet. <https://www.alphasense.com/wp-content/uploads/2013/06/COA4.pdf>  
 933
- 934 [61] Alphasense - AMETEK Inc.: NO2-A43F Nitrogen Dioxide Sensor - Datasheet.  
 935 <https://www.alphasense.com/wp-content/uploads/2013/07/NO2A43F.pdf>
- 936 [62] Alphasense - AMETEK Inc.: OX-A431 Oxidising Gas (O3+NO2) Sen-  
 937 sor - Datasheet. <https://www.alphasense.com/wp-content/uploads/2013/07/OXA431.pdf>  
 938
- 939 [63] Guangzhou Aosong Electronics Co., Ltd.: AM2302 (DHT22) Temperature and  
 940 Humidity Sensor Modules. <https://cdn.sparkfun.com/assets/f/7/d/9/c/DHT22.pdf>  
 941
- 942 [64] Spinelle, L., Gerboles, M., Villani, M.G., Aleixandre, M., Bonavitacola, F.: Field  
 943 calibration of a cluster of low-cost available sensors for air quality monitoring.  
 944 part a: Ozone and nitrogen dioxide. *Sensors and Actuators B: Chemical* **215**,  
 945 249–257 (2015)

- [65] Castell, N., Dauge, F.R., Schneider, P., Vogt, M., Lerner, U., Fishbain, B., Broday, D., Bartonova, A.: Can commercial low-cost sensor platforms contribute to air quality monitoring and exposure estimates? *Environment international* **99**, 293–302 (2017)
- [66] Boanini, C., Mecca, D., Pognant, F., Bo, M., Clerico, M.: Integrated mobile laboratory for air pollution assessment: Literature review and cc-TRAIRer design **12**(8), 1004 (2021) <https://doi.org/10.3390/atmos12081004> . Accessed 2024-11-26
- [67] Lewis, A., Peltier, W.R., Schneidmesser, E.: Low-cost sensors for the measurement of atmospheric composition: overview of topic and future applications (2018)
- [68] Neter, J., Kutner, M.H., Nachtsheim, C.J., Wasserman, W., et al.: *Applied linear statistical models* (1996)
- [69] Wood, S.N.: *Generalized Additive Models: an Introduction with R*. Chapman and Hall/CRC, ??? (2017)
- [70] Breiman, L.: Random forests. *Machine learning* **45**, 5–32 (2001)
- [71] Breiman, L.: Random forests. *Machine Learning* **45**(1), 5–32 (2001) <https://doi.org/10.1023/A:1010933404324>
- [72] Moore, D.S., Kirkland, S.: *The Basic Practice of Statistics* vol. 2. WH Freeman New York, ??? (2007)
- [73] Holstius, D.M., Pillarissetti, A., Smith, K., Seto, E.: Field calibrations of a low-cost aerosol sensor at a regulatory monitoring site in california. *Atmospheric Measurement Techniques* **7**(4), 1121–1131 (2014)
- [74] Mei, H., Han, P., Wang, Y., Zeng, N., Liu, D., Cai, Q., Deng, Z., Wang, Y., Pan, Y., Tang, X.: Field evaluation of low-cost particulate matter sensors in beijing. *Sensors* **20**(16), 4381 (2020)
- [75] Lopez-Restrepo, S., Yarce, A., Pinel, N., Quintero, O.L., Segers, A., Heemink, A.W.: Urban air quality modeling using low-cost sensor network and data assimilation in the aburrá valley, colombia. *Atmosphere* **12**(1), 91 (2021)
- [76] Bisignano, A., Carotenuto, F., Zaldei, A., Giovannini, L.: Field calibration of a low-cost sensors network to assess traffic-related air pollution along the brenner highway. *Atmospheric Environment* **275**, 119008 (2022)
- [77] Chang, J.C., Hanna, S.R.: Air quality model performance evaluation. *Meteorology and Atmospheric Physics* **87**(1), 167–196 (2004)

- 980 [78] European Parliament and Council: Directive 2008/50/EC of the European Par-  
981 liament and of the Council of 21 May 2008 on ambient air quality and cleaner air  
982 for Europe.  
983 <https://eur-lex.europa.eu/eli/dir/2008/50/oj/eng> (2008)

ARTICLE IN PRESS